

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021622\
 Data File : VV024702.D
 Acq On : 16 Feb 2022 17:27
 Operator : SY/MD
 Sample : N1510-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4M73

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV024702.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	96	rVB	53371	53085	12.12%	1.574%
2	1.568	157	164	176	rBV	56022	62493	14.27%	1.853%
3	2.111	322	333	345	rBV	99120	142493	32.54%	4.226%
4	3.895	876	888	934	rBV	46427	166246	37.96%	4.930%
5	4.349	1013	1029	1055	rBV	82964	215826	49.28%	6.401%
6	5.050	1231	1247	1279	rBV3	162969	412520	94.19%	12.234%
7	5.619	1413	1424	1451	rBV2	99238	202063	46.14%	5.993%
8	5.915	1504	1516	1532	rBV5	4486	9955	2.27%	0.295%
9	6.069	1552	1564	1586	rBV	97449	200711	45.83%	5.952%
10	6.989	1840	1850	1882	rBV	46369	87447	19.97%	2.593%
11	7.317	1940	1952	1968	rBV	188824	327516	74.78%	9.713%
12	7.394	1968	1976	1992	rVB	22023	41271	9.42%	1.224%
13	7.625	2037	2048	2071	rBV2	26572	48996	11.19%	1.453%
14	8.088	2182	2192	2229	rBV	221871	437948	100.00%	12.988%
15	8.853	2419	2430	2455	rBV	163296	271535	62.00%	8.053%
16	10.213	2840	2853	2871	rBV	67248	105914	24.18%	3.141%
17	10.381	2896	2905	2915	rVB4	4079	6409	1.46%	0.190%
18	11.249	3164	3175	3191	rBV	185652	284260	64.91%	8.430%
19	11.622	3280	3291	3306	rBV	184970	289393	66.08%	8.582%
20	14.036	4030	4042	4053	rBV	3388	5822	1.33%	0.173%




Sum of corrected areas: 3371903

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021622\
Data File : VV024702.D
Acq On : 16 Feb 2022 17:27
Operator : SY/MD
Sample : N1510-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4M73

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

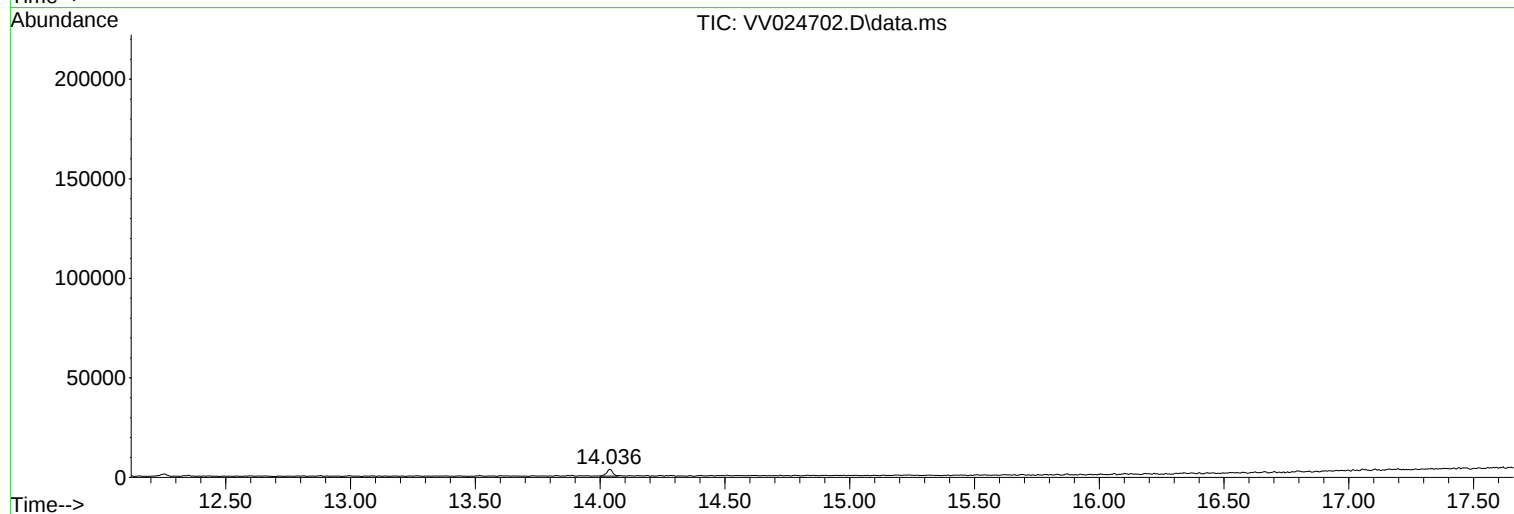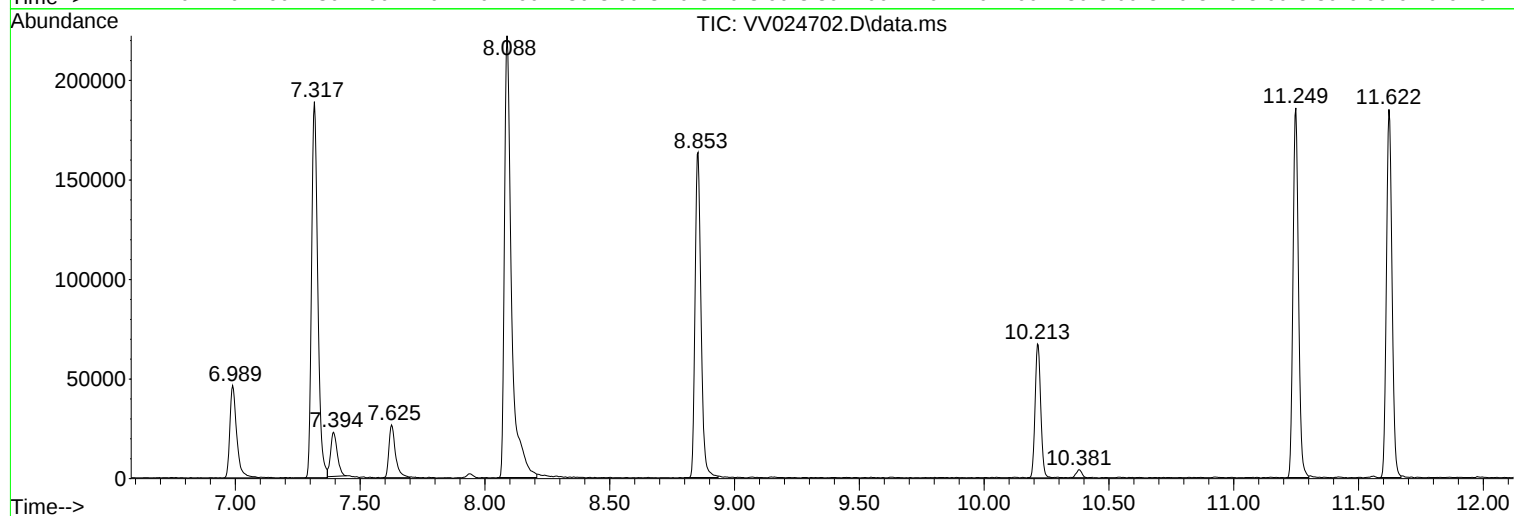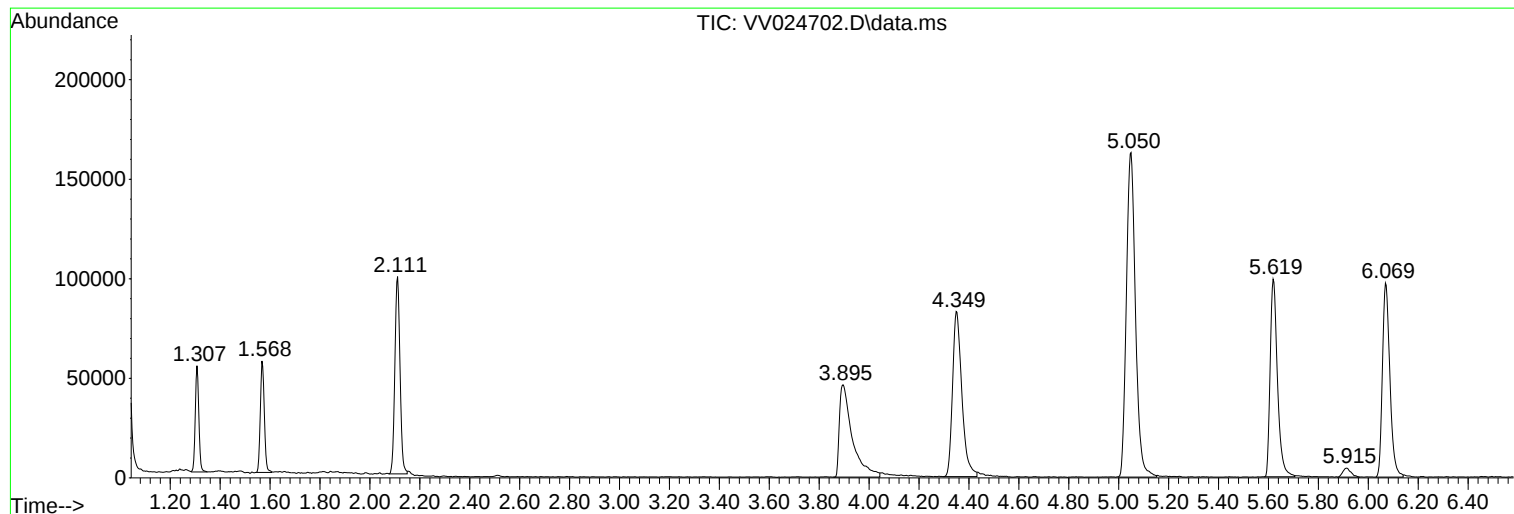

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021622\
Data File : VV024702.D
Acq On : 16 Feb 2022 17:27
Operator : SY/MD
Sample : N1510-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4M73

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021622\
Data File : VV024702.D
Acq On : 16 Feb 2022 17:27
Operator : SY/MD
Sample : N1510-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4M73

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc