

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021622\
 Data File : VV024703.D
 Acq On : 16 Feb 2022 17:50
 Operator : SY/MD
 Sample : N1510-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4M00

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV024703.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.117	20	24	31	rVB	6837	6397	1.39%	0.184%
2	1.294	69	79	90	rBV2	72747	102468	22.28%	2.945%
3	1.404	105	113	120	rBV3	2728	5284	1.15%	0.152%
4	1.558	153	161	172	rBV	62749	70444	15.32%	2.024%
5	2.098	319	329	348	rVB	117360	168018	36.54%	4.828%
6	2.281	368	386	398	rBV5	3711	12623	2.75%	0.363%
7	3.690	812	824	836	rBV5	2098	5625	1.22%	0.162%
8	3.969	892	911	963	rBV2	25438	132290	28.77%	3.802%
9	4.346	1011	1028	1054	rBV	83752	211950	46.09%	6.091%
10	5.043	1229	1245	1274	rBV2	195568	459823	100.00%	13.214%
11	5.616	1410	1423	1451	rBV	108988	219486	47.73%	6.307%
12	5.902	1504	1512	1531	rVB5	4264	9331	2.03%	0.268%
13	6.069	1547	1564	1585	rBV2	108363	219862	47.81%	6.318%
14	6.985	1839	1849	1868	rBV2	48079	88820	19.32%	2.552%
15	7.313	1939	1951	1971	rBV	216909	380001	82.64%	10.920%
16	7.394	1971	1976	1985	rVB2	2813	5275	1.15%	0.152%
17	7.625	2039	2048	2069	rBV	26747	46934	10.21%	1.349%
18	8.098	2185	2195	2207	rBV	154184	290832	63.25%	8.358%
19	8.850	2418	2429	2453	rBV	170986	285411	62.07%	8.202%
20	9.101	2499	2507	2517	rBV2	4243	5759	1.25%	0.165%
21	10.217	2844	2854	2867	rBV	61443	95864	20.85%	2.755%
22	11.249	3161	3175	3196	rVB	183980	292567	63.63%	8.408%
23	11.532	3255	3263	3279	rVB3	6846	12644	2.75%	0.363%
24	11.622	3279	3291	3306	rBV	203838	314894	68.48%	9.049%
25	12.345	3507	3516	3526	rBV4	4105	6039	1.31%	0.174%
26	13.628	3905	3915	3925	rVB5	5859	8254	1.80%	0.237%
27	13.747	3942	3952	3962	rBV3	5871	9196	2.00%	0.264%
28	14.040	4033	4043	4052	rVB2	4016	6373	1.39%	0.183%
29	15.110	4369	4376	4384	rBV6	5135	7367	1.60%	0.212%




Sum of corrected areas: 3479831

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021622\
Data File : VV024703.D
Acq On : 16 Feb 2022 17:50
Operator : SY/MD
Sample : N1510-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4M00

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

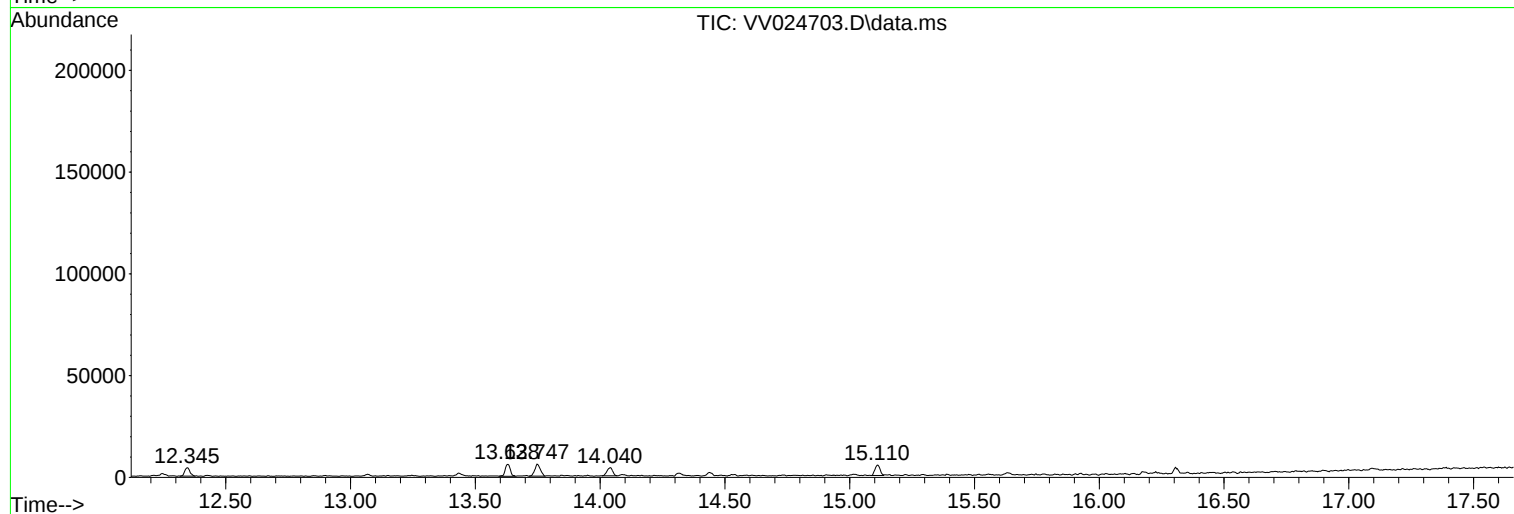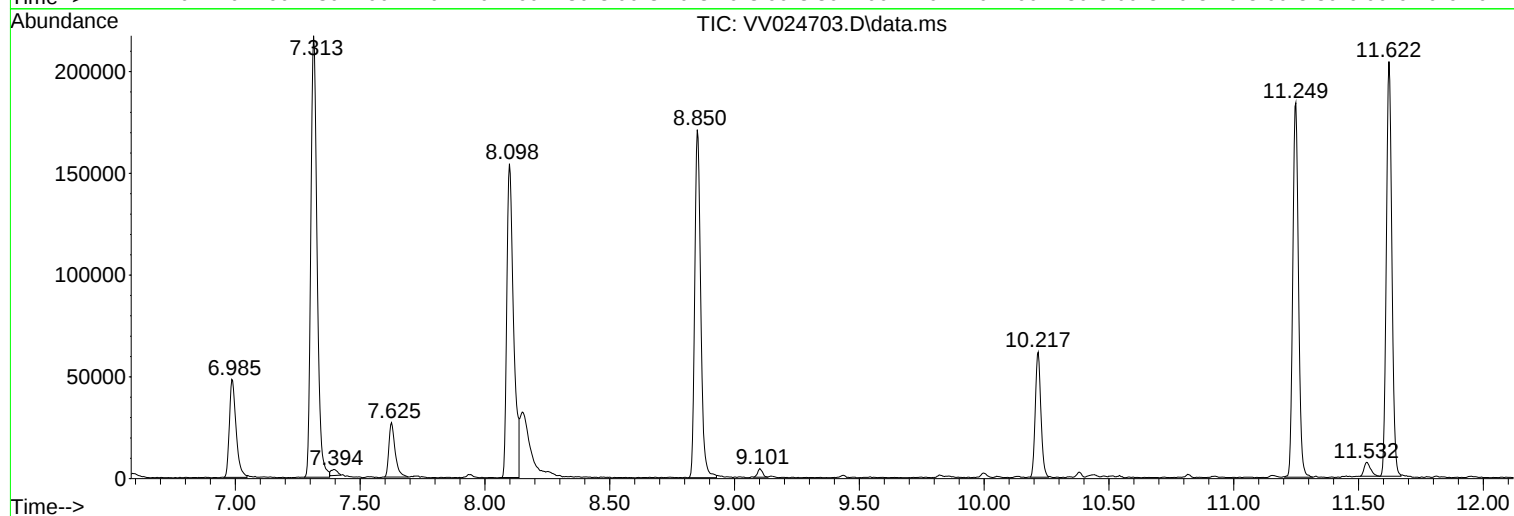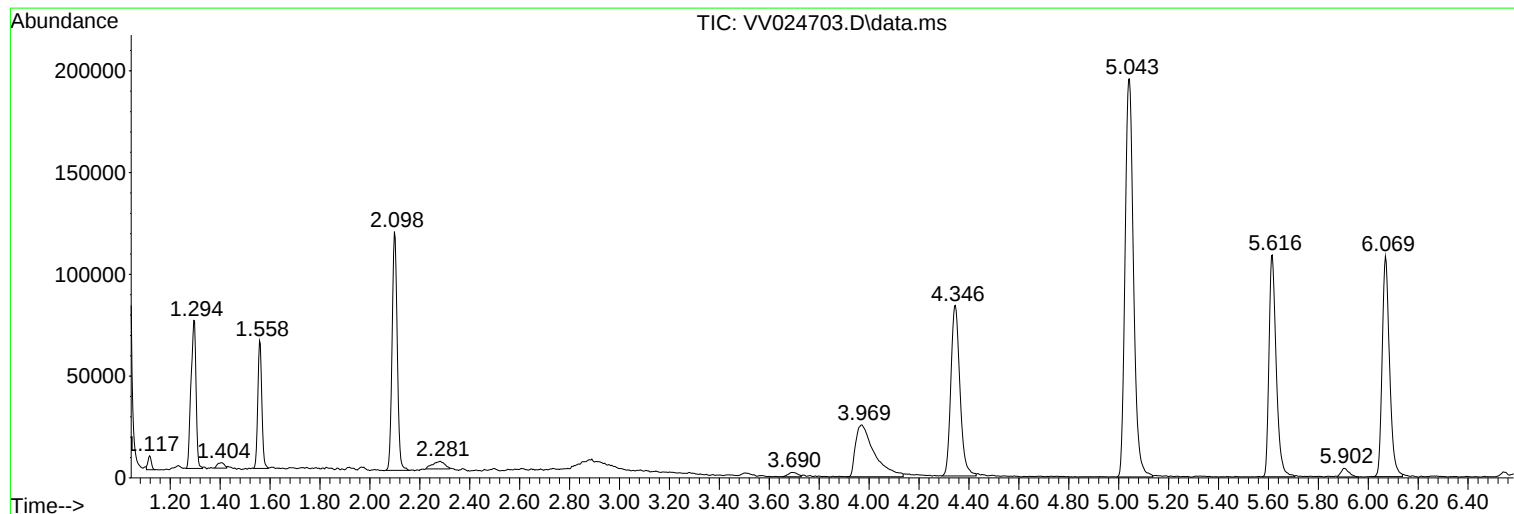

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021622\
Data File : VV024703.D
Acq On : 16 Feb 2022 17:50
Operator : SY/MD
Sample : N1510-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4M00

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021622\
Data File : VV024703.D
Acq On : 16 Feb 2022 17:50
Operator : SY/MD
Sample : N1510-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4M00

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc