

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021622\
 Data File : VV024708.D
 Acq On : 16 Feb 2022 19:47
 Operator : SY/MD
 Sample : N1510-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4M24

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV024708.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	93	rVB	64540	65912	13.75%	1.735%
2	1.571	157	165	175	rBV	65554	74428	15.52%	1.959%
3	2.111	321	333	347	rVB	122520	176280	36.76%	4.640%
4	3.899	879	889	938	rBV2	43818	172837	36.04%	4.549%
5	4.349	1013	1029	1054	rBV	86263	216517	45.15%	5.699%
6	5.050	1231	1247	1276	rBV2	192194	479519	100.00%	12.621%
7	5.619	1412	1424	1449	rBV	118813	242332	50.54%	6.378%
8	6.069	1551	1564	1588	rBV	113398	233383	48.67%	6.143%
9	6.989	1839	1850	1870	rBV	51504	96635	20.15%	2.543%
10	7.317	1940	1952	1971	rBV	225551	391618	81.67%	10.307%
11	7.394	1973	1976	1991	rVB3	3611	6698	1.40%	0.176%
12	7.625	2039	2048	2069	rBV2	28538	51471	10.73%	1.355%
13	8.088	2181	2192	2228	rBV	227210	449026	93.64%	11.818%
14	8.854	2416	2430	2459	rBV	191737	321250	66.99%	8.455%
15	10.214	2842	2853	2873	rBV	75381	119156	24.85%	3.136%
16	11.246	3163	3174	3196	rBV	214296	327965	68.39%	8.632%
17	11.622	3280	3291	3310	rBV	217621	336406	70.15%	8.854%
18	14.040	4032	4043	4056	rBV2	7110	11518	2.40%	0.303%
19	16.178	4697	4708	4718	rBV5	13946	19950	4.16%	0.525%
20	16.304	4742	4747	4760	rVB6	4246	6559	1.37%	0.173%




Sum of corrected areas: 3799460

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021622\
Data File : VV024708.D
Acq On : 16 Feb 2022 19:47
Operator : SY/MD
Sample : N1510-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4M24

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

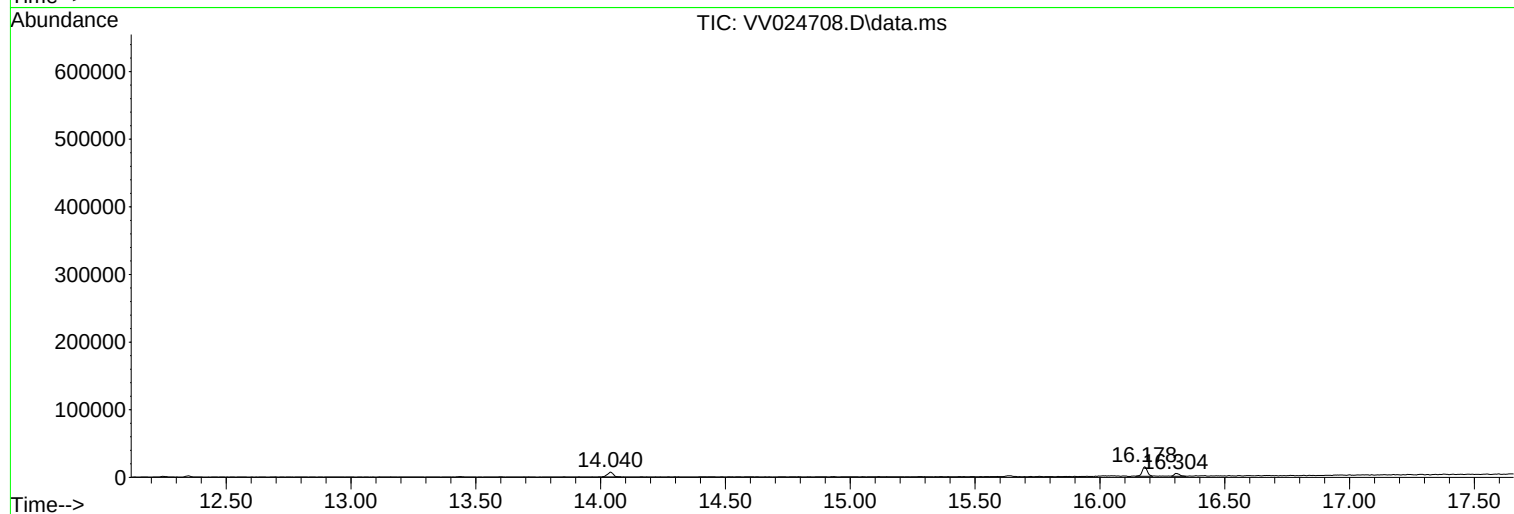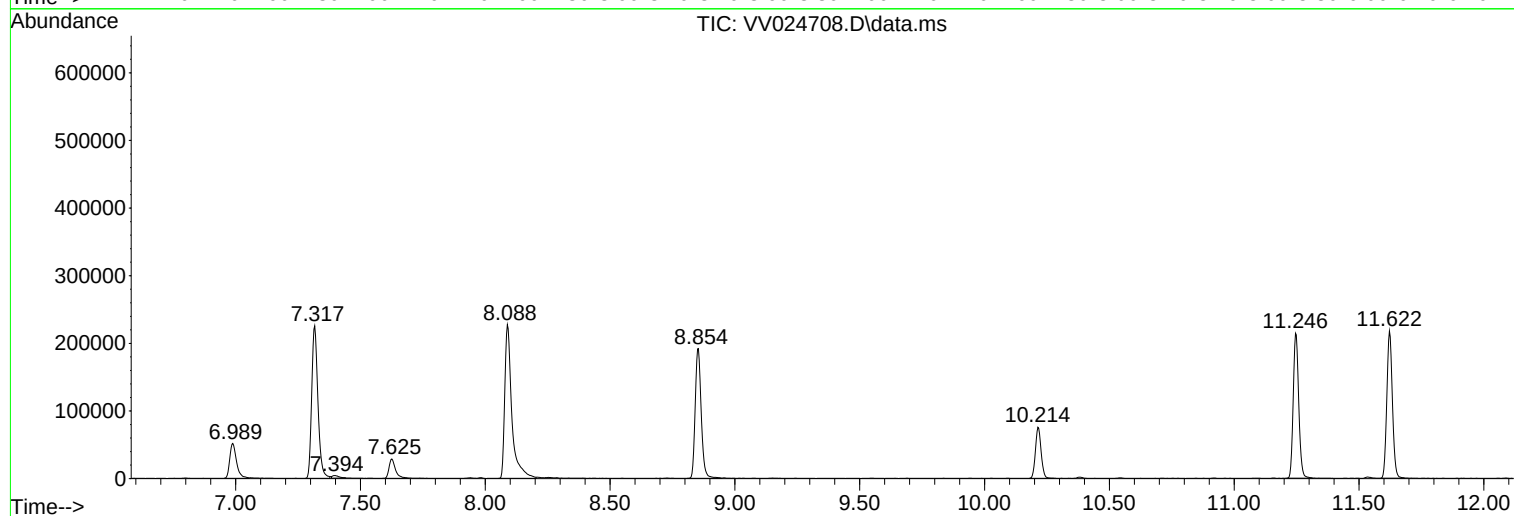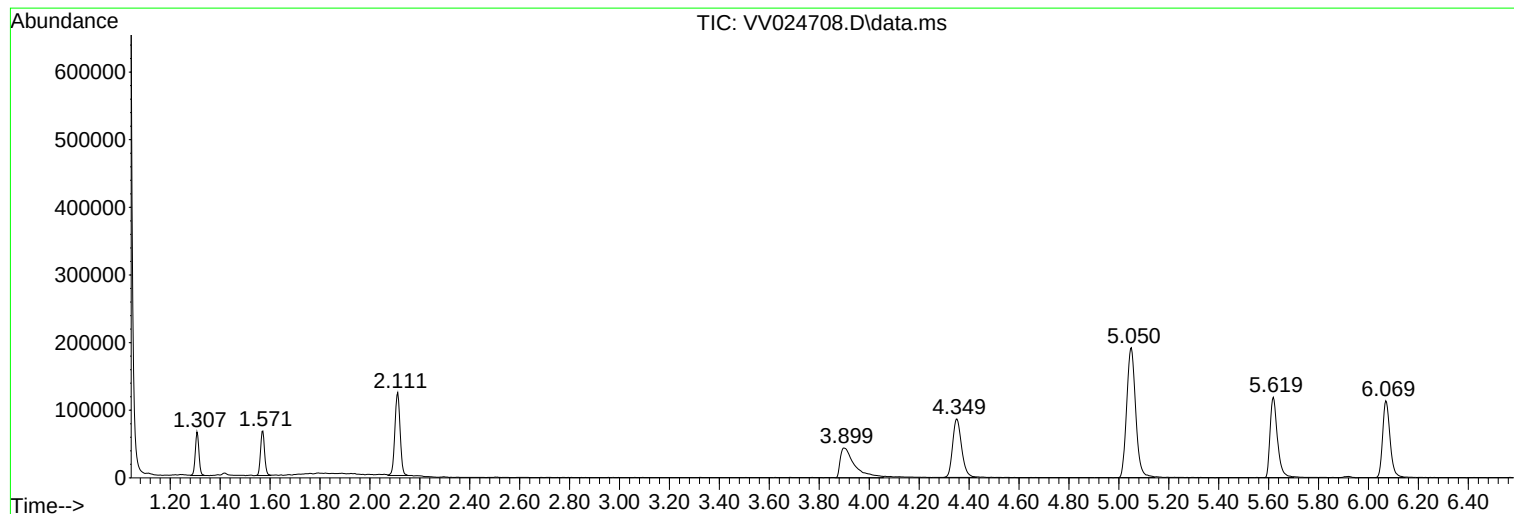

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021622\
Data File : VV024708.D
Acq On : 16 Feb 2022 19:47
Operator : SY/MD
Sample : N1510-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4M24

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021622\
Data File : VV024708.D
Acq On : 16 Feb 2022 19:47
Operator : SY/MD
Sample : N1510-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4M24

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
