


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021622\
 Data File : VV024691.D
 Acq On : 16 Feb 2022 10:19
 Operator : SY/MD
 Sample : BFB271
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB271

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Wed Feb 16 23:36:08 2022

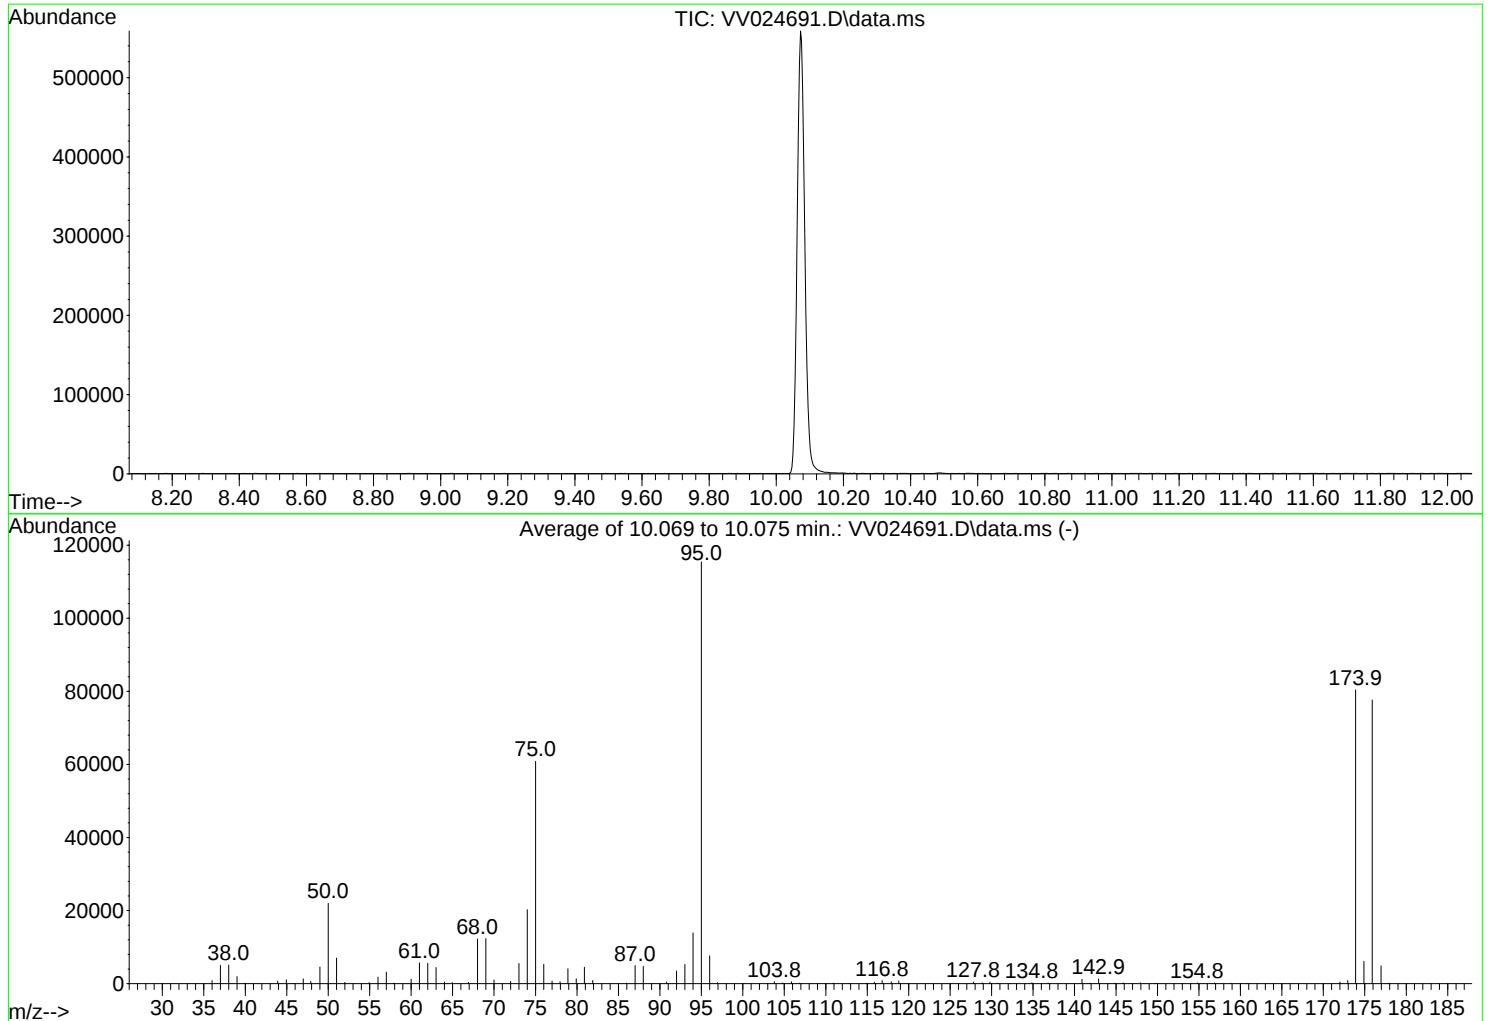

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	21989	PASS
75	95	30	80	52.7	60845	PASS
95	95	100	100	100.0	115440	PASS
96	95	5	9	6.6	7614	PASS
173	174	0.00	2	1.0	841	PASS
174	95	50	120	69.7	80408	PASS
175	174	5	9	7.6	6105	PASS
176	174	95	105	96.5	77621	PASS
177	176	5	10	6.3	4882	PASS

m/z	Abundance
39.90	115.0
43.90	292.0

Instrument :
MSVOA_V
ClientSampleId :
BFB271

m/z	Abundance
36.00	842.0
37.00	4949.0
38.00	4845.0
39.00	2002.0
40.00	195.0
44.00	964.0
45.00	1085.0
45.90	130.0
47.00	1364.0
47.90	583.0
49.00	4464.0
50.00	21432.0
51.00	6778.0
52.00	332.0
54.90	283.0
56.00	1742.0
57.00	3120.0
57.90	142.0
60.00	1123.0
61.00	5442.0
62.00	5390.0
63.00	4245.0
64.00	474.0
65.00	328.0
66.90	314.0
68.00	11838.0
69.00	11969.0
70.00	957.0
72.00	647.0
73.00	5412.0
74.00	19272.0
75.00	59072.0
76.00	5042.0
77.00	692.0
78.00	507.0
78.90	3940.0
79.90	1316.0
80.90	4252.0
81.90	793.0
86.00	147.0
87.00	4642.0
88.00	4591.0
90.80	430.0
92.00	3346.0
93.00	5065.0
94.00	13329.0
95.00	111272.0
96.00	7455.0
97.00	223.0
103.80	567.0
104.80	159.0
105.80	456.0
106.90	116.0
110.90	125.0
112.80	106.0
114.80	144.0
115.80	417.0
116.80	845.0
117.90	457.0
118.80	686.0
127.80	390.0
128.90	175.0
129.80	396.0
130.80	148.0
134.90	205.0
136.80	185.0
140.90	1054.0
141.80	114.0
142.90	1121.0
144.80	112.0
145.80	251.0
148.00	216.0
149.80	110.0
154.80	190.0
156.90	188.0
158.80	146.0
172.00	366.0
172.90	763.0
173.90	75280.0
174.90	5790.0
175.90	71904.0
177.00	4592.0
177.90	157.0

Instrument :
MSVOA_V
ClientSampleId :
BFB271

m/z	Abundance
36.00	853.0
37.00	5139.0
38.00	5215.0
39.00	2000.0
40.00	223.0
44.00	1038.0
45.00	1105.0
45.80	106.0
47.00	1371.0
47.90	616.0
49.00	4629.0
50.00	22696.0
51.00	7226.0
52.00	346.0
55.00	316.0
56.00	1868.0
57.00	3257.0
57.90	150.0
60.00	1310.0
61.00	5881.0
62.00	5712.0
63.00	4555.0
64.00	425.0
64.90	303.0
66.90	351.0
68.00	12605.0
69.00	12658.0
70.00	1032.0
72.00	597.0
73.00	5724.0
74.00	20872.0
75.00	62784.0
76.00	5471.0
77.00	725.0
77.90	533.0
78.90	4205.0
79.90	1401.0
80.90	4684.0
81.90	869.0
86.00	167.0
87.00	5212.0
88.00	4817.0
90.80	464.0
92.00	3549.0
93.00	5406.0
94.00	14418.0
95.00	119336.0
96.00	7897.0
97.00	262.0
103.80	569.0
104.80	193.0
105.80	535.0
106.80	146.0
110.90	145.0
114.90	105.0
115.80	410.0
116.80	883.0
117.90	521.0
118.80	785.0
127.80	445.0
128.80	201.0
129.80	398.0
130.70	157.0
134.90	210.0
136.80	185.0
140.90	1222.0
141.80	131.0
142.90	1359.0
144.80	145.0
145.80	246.0
148.00	228.0
149.80	102.0
154.80	255.0
156.90	226.0
158.90	154.0
172.00	466.0
172.90	858.0
173.90	83176.0
174.90	6368.0
175.90	80456.0
176.90	5046.0
177.90	155.0

Instrument :
MSVOA_V
ClientSampleId :
BFB271

m/z	Abundance
36.00	790.0
37.00	4880.0
38.00	5135.0
39.00	1780.0
39.90	237.0
43.90	1029.0
44.90	978.0
47.00	1278.0
47.90	616.0
49.00	4591.0
50.00	21840.0
51.00	7073.0
52.00	317.0
55.00	339.0
56.00	1831.0
57.00	3076.0
57.90	138.0
60.00	1287.0
61.00	5759.0
62.00	5576.0
63.00	4473.0
64.00	360.0
64.90	284.0
66.90	382.0
68.00	12192.0
69.00	12428.0
70.00	1006.0
72.00	550.0
73.00	5403.0
74.00	20584.0
75.00	60680.0
76.00	5351.0
77.00	662.0
77.90	485.0
78.90	4060.0
79.90	1218.0
80.90	4414.0
81.90	910.0
85.90	181.0
87.00	5044.0
88.00	4748.0
90.80	429.0
92.00	3494.0
93.00	5254.0
94.00	13942.0
95.00	115712.0
96.00	7490.0
96.90	285.0
103.80	488.0
104.80	208.0
105.90	572.0
106.80	177.0
110.90	138.0
115.90	416.0
116.80	819.0
117.90	537.0
118.80	729.0
127.80	458.0
128.80	236.0
129.80	383.0
130.80	157.0
134.80	217.0
136.80	166.0
140.90	1216.0
141.90	140.0
142.90	1386.0
144.90	173.0
145.90	193.0
147.90	229.0
154.80	280.0
156.90	240.0
158.90	135.0
160.80	113.0
172.00	516.0
173.00	903.0
173.90	82768.0
174.90	6157.0
175.90	80504.0
176.90	5009.0
177.90	150.0

Instrument :
MSVOA_V
ClientSampleId :
BFB271