

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021624\
 Data File : VV034221.D
 Acq On : 16 Feb 2024 16:49
 Operator : SY/MD
 Sample : P1498-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AE5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV034221.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	65	74	86	rVB	11784	14042	7.50%	1.041%
2	1.490	118	140	144	rBV	5492	14948	7.98%	1.108%
3	1.523	145	150	162	rVB	16636	21129	11.29%	1.567%
4	2.056	307	316	330	rVB	26865	39502	21.10%	2.929%
5	2.449	430	438	450	rBV2	2149	3221	1.72%	0.239%
6	3.796	848	857	885	rBV2	23902	70041	37.41%	5.193%
7	4.252	986	999	1026	rBV2	18532	50926	27.20%	3.776%
8	4.735	1137	1149	1167	rBB3	5760	14523	7.76%	1.077%
9	4.960	1205	1219	1245	rBV4	40481	104487	55.81%	7.747%
10	5.535	1388	1398	1429	rBV	68056	140906	75.26%	10.447%
11	5.844	1484	1494	1512	rVB5	8870	19019	10.16%	1.410%
12	5.992	1530	1540	1564	rBV2	22631	48245	25.77%	3.577%
13	6.921	1820	1829	1849	rBV2	10385	21478	11.47%	1.592%
14	7.246	1920	1930	1946	rBV	43364	77911	41.62%	5.777%
15	7.564	2021	2029	2047	rBV4	6420	12149	6.49%	0.901%
16	7.905	2126	2135	2153	rVB	47156	80861	43.19%	5.995%
17	8.027	2165	2173	2215	rBV	91074	187214	100.00%	13.881%
18	8.786	2399	2409	2436	rBV	99689	168209	89.85%	12.472%
19	10.156	2825	2835	2850	rBV2	26186	41096	21.95%	3.047%
20	11.188	3146	3156	3171	rBV	89894	145570	77.76%	10.793%
21	11.564	3262	3273	3286	rBV	46348	73237	39.12%	5.430%




Sum of corrected areas: 1348714

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021624\
Data File : VV034221.D
Acq On : 16 Feb 2024 16:49
Operator : SY/MD
Sample : P1498-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

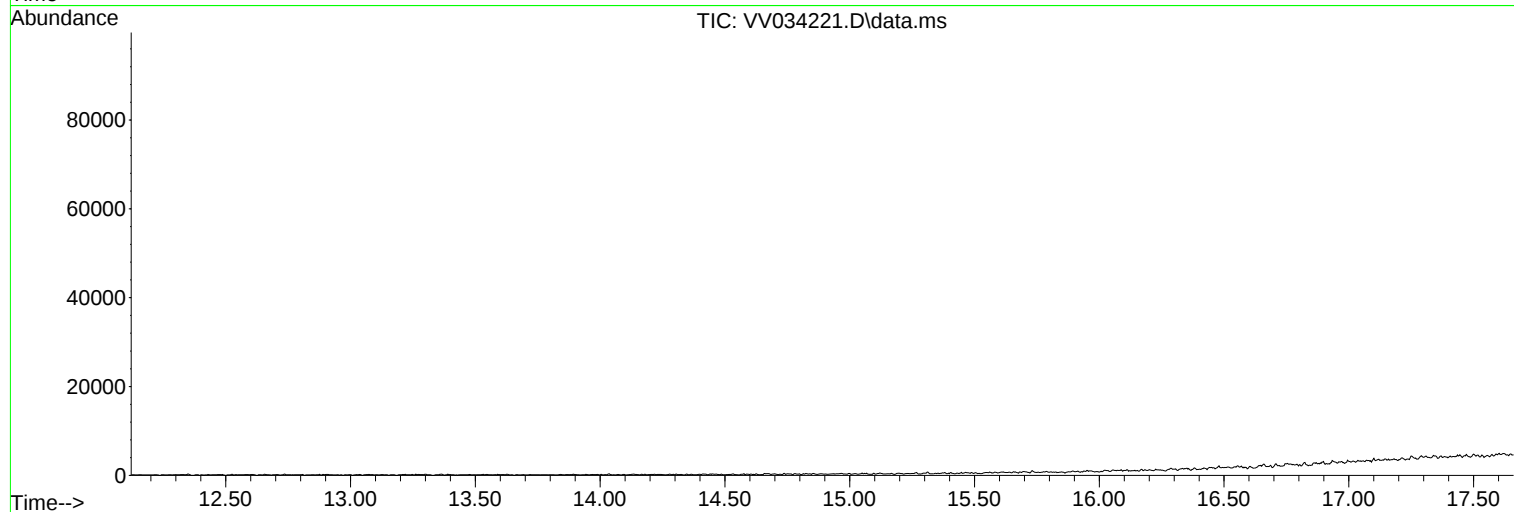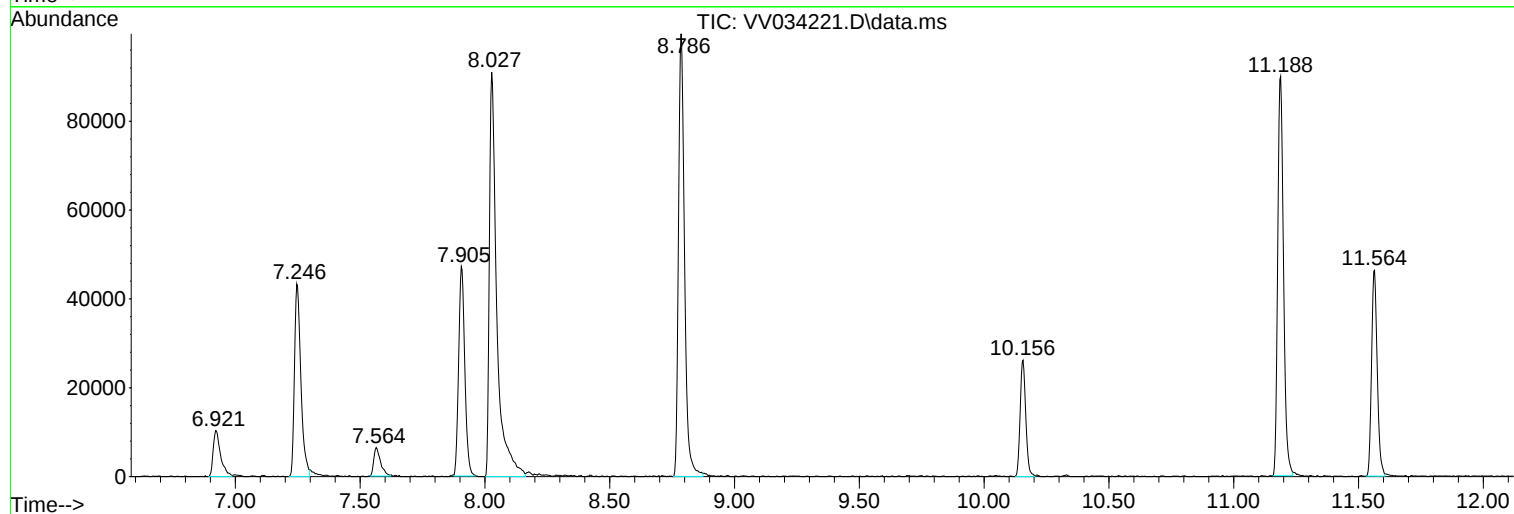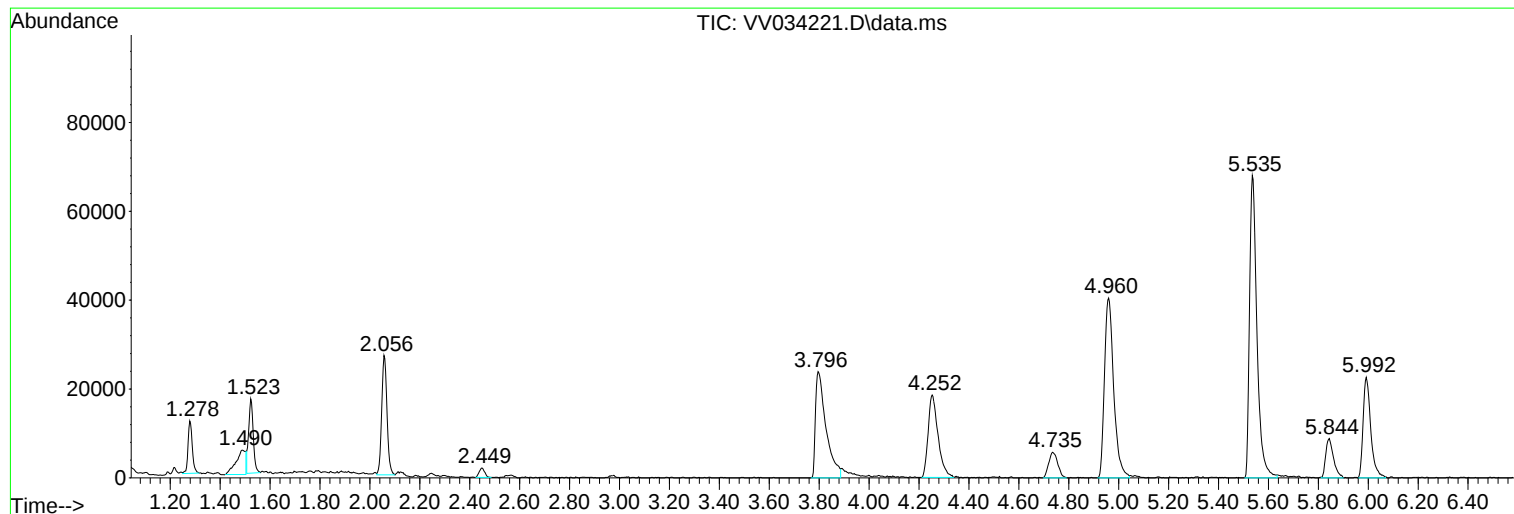

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021624\
Data File : VV034221.D
Acq On : 16 Feb 2024 16:49
Operator : SY/MD
Sample : P1498-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021624\
Data File : VV034221.D
Acq On : 16 Feb 2024 16:49
Operator : SY/MD
Sample : P1498-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc