


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021624\
Data File : VV034205.D
Acq On : 16 Feb 2024 08:21
Operator : SY/MD
Sample : BFB254
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB254

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Tue Feb 20 01:47:35 2024

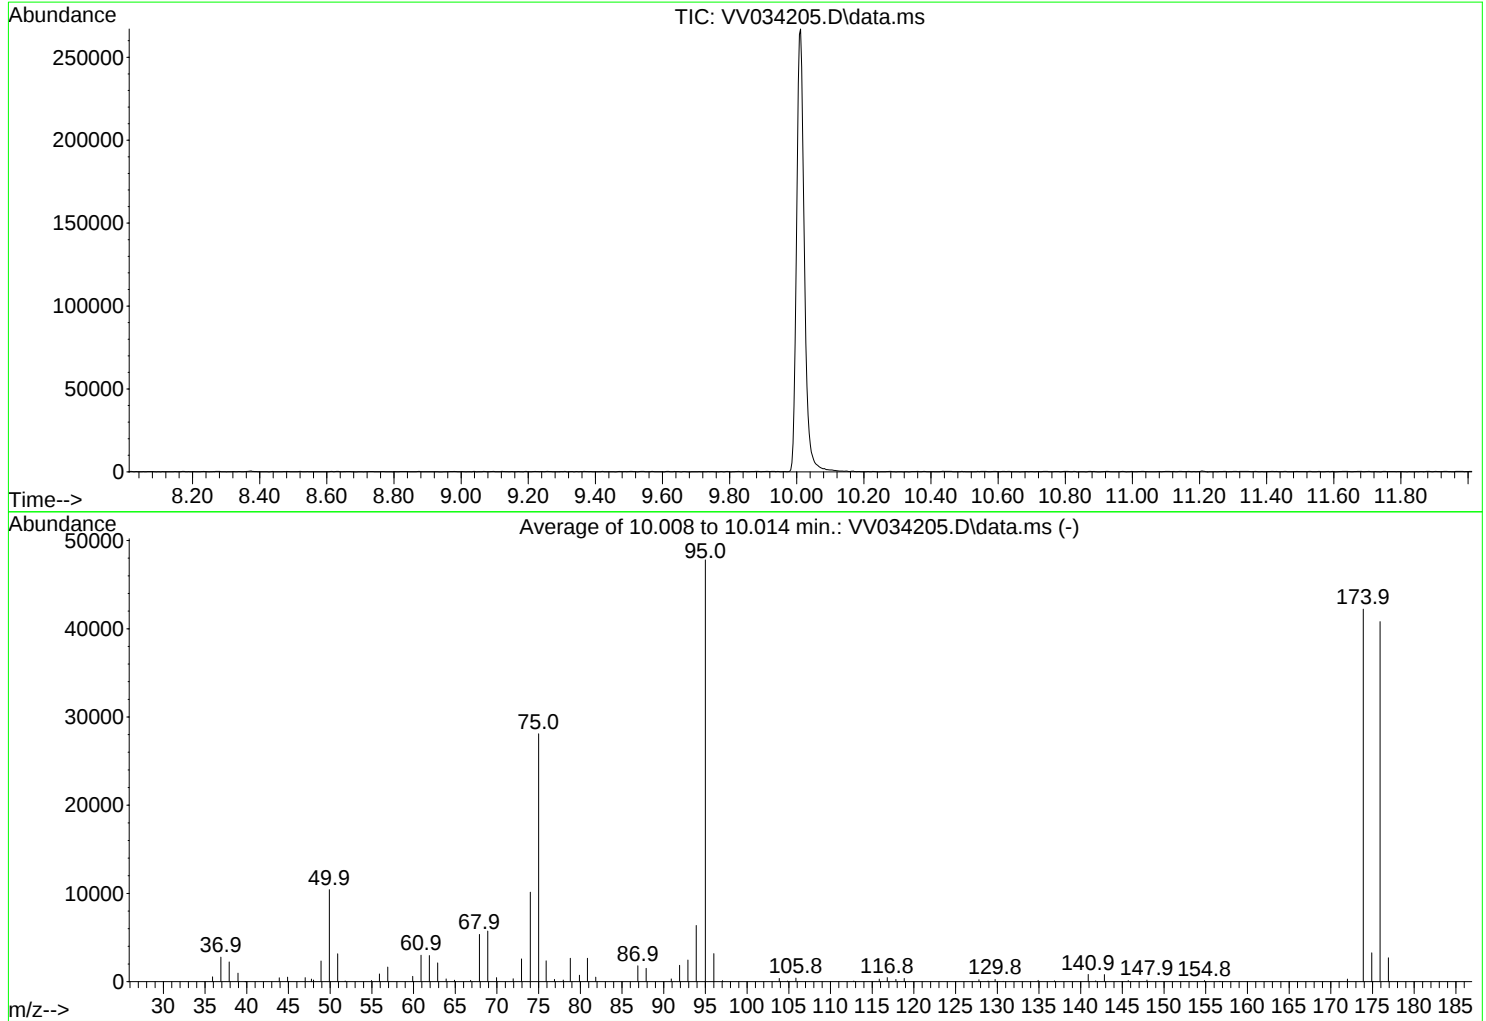

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2777

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.8	10434	PASS
75	95	30	80	58.8	28093	PASS
95	95	100	100	100.0	47811	PASS
96	95	5	9	6.6	3173	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	88.3	42216	PASS
175	174	5	9	7.7	3264	PASS
176	174	95	105	96.7	40811	PASS
177	176	5	10	6.6	2705	PASS

m/z	Abundance
39.90	136.0

Instrument :
MSVOA_V
ClientSampleId :
BFB254

m/z	Abundance
35.90	530.0
36.90	2769.0
37.90	2326.0
38.90	1054.0
39.80	134.0
43.90	431.0
44.90	497.0
47.00	472.0
47.80	287.0
48.90	2375.0
49.90	11052.0
50.90	3286.0
55.00	109.0
55.90	928.0
56.90	1748.0
59.90	568.0
60.90	2970.0
61.90	3116.0
62.90	2259.0
63.90	311.0
64.90	172.0
66.80	146.0
67.90	5721.0
68.90	6060.0
69.90	462.0
72.00	258.0
72.90	2605.0
74.00	10503.0
75.00	29112.0
75.90	2520.0
76.90	248.0
78.00	198.0
78.80	2749.0
79.90	798.0
80.80	2701.0
81.80	495.0
86.90	1858.0
87.90	1600.0
90.90	313.0
91.90	1918.0
92.90	2570.0
93.90	6525.0
95.00	48856.0
96.00	3389.0
97.00	115.0
103.80	373.0
104.90	111.0
105.80	419.0
112.80	121.0
115.90	268.0
116.80	484.0
117.80	238.0
118.80	339.0
127.80	211.0
129.70	231.0
134.90	144.0
136.90	133.0
140.90	825.0
142.80	805.0
145.60	123.0
148.00	160.0
154.80	123.0
156.70	105.0
172.00	246.0
173.90	42376.0
174.90	3397.0
175.90	40824.0
176.90	2669.0

Instrument :
MSVOA_V
ClientSampleId :
BFB254

m/z	Abundance
35.90	558.0
36.90	2848.0
37.90	2286.0
39.00	1007.0
39.80	151.0
43.90	436.0
44.90	529.0
47.00	479.0
47.70	297.0
48.00	276.0
48.90	2404.0
49.90	10772.0
50.90	3288.0
51.80	117.0
55.00	126.0
55.90	861.0
56.90	1690.0
59.90	616.0
60.90	3116.0
61.90	3034.0
62.90	2155.0
63.90	342.0
64.90	170.0
66.90	143.0
67.90	5483.0
68.90	5860.0
69.90	463.0
71.90	311.0
72.90	2653.0
74.00	10490.0
75.00	29024.0
75.90	2400.0
76.90	257.0
78.00	189.0
78.80	2750.0
79.90	757.0
80.90	2733.0
81.90	511.0
86.90	1910.0
87.90	1508.0
90.90	335.0
91.90	1961.0
92.90	2512.0
93.90	6533.0
95.00	49552.0
96.00	3282.0
97.00	116.0
103.80	368.0
104.80	106.0
105.90	418.0
112.80	118.0
115.80	297.0
116.80	460.0
117.80	246.0
118.90	380.0
127.80	221.0
128.90	105.0
129.80	269.0
134.90	154.0
136.80	120.0
140.90	834.0
141.80	139.0
142.90	818.0
145.70	123.0
147.90	184.0
154.80	124.0
172.00	309.0
173.90	43656.0
174.90	3378.0
175.90	42152.0
176.90	2807.0

Instrument :
MSVOA_V
ClientSampleId :
BFB254

m/z	Abundance
35.90	527.0
36.90	2687.0
37.90	2084.0
39.00	842.0
39.80	149.0
43.90	430.0
44.90	486.0
47.00	422.0
47.70	267.0
48.00	275.0
48.90	2253.0
49.90	9478.0
50.90	2917.0
51.80	119.0
54.90	141.0
55.90	806.0
56.90	1509.0
59.90	593.0
60.90	2924.0
61.90	2722.0
62.90	1941.0
63.90	287.0
64.90	137.0
66.90	151.0
67.90	4873.0
68.90	5257.0
70.00	447.0
71.90	384.0
73.00	2462.0
74.00	9428.0
75.00	26144.0
75.90	2163.0
76.90	259.0
77.80	148.0
78.80	2460.0
79.90	615.0
80.90	2504.0
81.90	494.0
86.90	1644.0
87.90	1399.0
90.90	297.0
91.90	1675.0
92.90	2252.0
93.90	6052.0
95.00	45024.0
96.00	2847.0
97.10	113.0
103.90	357.0
105.90	383.0
115.80	316.0
116.80	423.0
117.90	257.0
118.90	390.0
127.80	209.0
128.90	116.0
129.80	266.0
130.70	104.0
134.90	128.0
140.90	777.0
141.80	126.0
142.90	747.0
145.80	119.0
147.90	183.0
154.90	121.0
172.00	306.0
173.90	40616.0
174.90	3017.0
175.90	39456.0
176.90	2639.0

Instrument :
MSVOA_V
ClientSampleId :
BFB254