

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021722\
 Data File : VV024742.D
 Acq On : 17 Feb 2022 23:07
 Operator : SY/MD
 Sample : N1522-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4M92

Quant Time: Feb 18 07:38:21 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Feb 18 07:32:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	167090	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	156530	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	69648	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	65500	4.622	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	92.400%	
7) Chloroethane-d5	1.568	69	55141	4.743	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	94.800%	
11) 1,1-Dichloroethene-d2	2.111	63	89312	3.439	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	68.800%	
20) 2-Butanone-d5	3.889	46	114687	56.654	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	113.300%	
24) Chloroform-d	4.352	84	103425	4.677	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	93.600%	
26) 1,2-Dichloroethane-d4	5.034	65	50637	5.137	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	102.800%	
32) Benzene-d6	5.053	84	215393	4.770	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	95.400%	
36) 1,2-Dichloropropane-d6	6.069	67	66343	4.992	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	99.800%	
41) Toluene-d8	7.317	98	189609	4.621	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	92.400%	
43) trans-1,3-Dichloroprop...	7.622	79	21006	4.745	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	94.800%	
46) 2-Hexanone-d5	8.088	63	92363	53.022	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	106.040%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	37556	4.689	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	93.800%	
66) 1,2-Dichlorobenzene-d4	11.622	152	59638	4.949	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	99.000%	
Target Compounds						Qvalue
8) Chloroethane	1.310	64	956	0.087	ug/L #	1
13) Acetone	2.182	43	5744	4.024	ug/L	98
22) cis-1,2-Dichloroethene	3.924	96	1268	0.094	ug/L	74
25) Chloroform	4.381	83	4791	0.197	ug/L	97
35) Methylcyclohexane	6.072	83	16264	0.717	ug/L #	20
37) 1,2-Dichloropropane	6.178	63	6916	0.552	ug/L #	89
39) cis-1,3-Dichloropropene	6.982	75	1494	0.086	ug/L #	73
42) Toluene	7.387	91	1825767	32.358	ug/L	98
52) Ethylbenzene	9.017	91	5104	0.083	ug/L	98
53) m,p-xylene	9.143	106	6622	0.284	ug/L	88
54) o-xylene	9.548	106	2661	0.117	ug/L	99
55) Styrene	9.570	104	2798	0.076	ug/L	98
61) 1,2,3-Trichloropropane	11.246	75	9121	1.445	ug/L #	68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021722\
Data File : VV024742.D
Acq On : 17 Feb 2022 23:07
Operator : SY/MD
Sample : N1522-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4M92

Quant Time: Feb 18 07:38:21 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Feb 18 07:32:51 2022
Response via : Initial Calibration




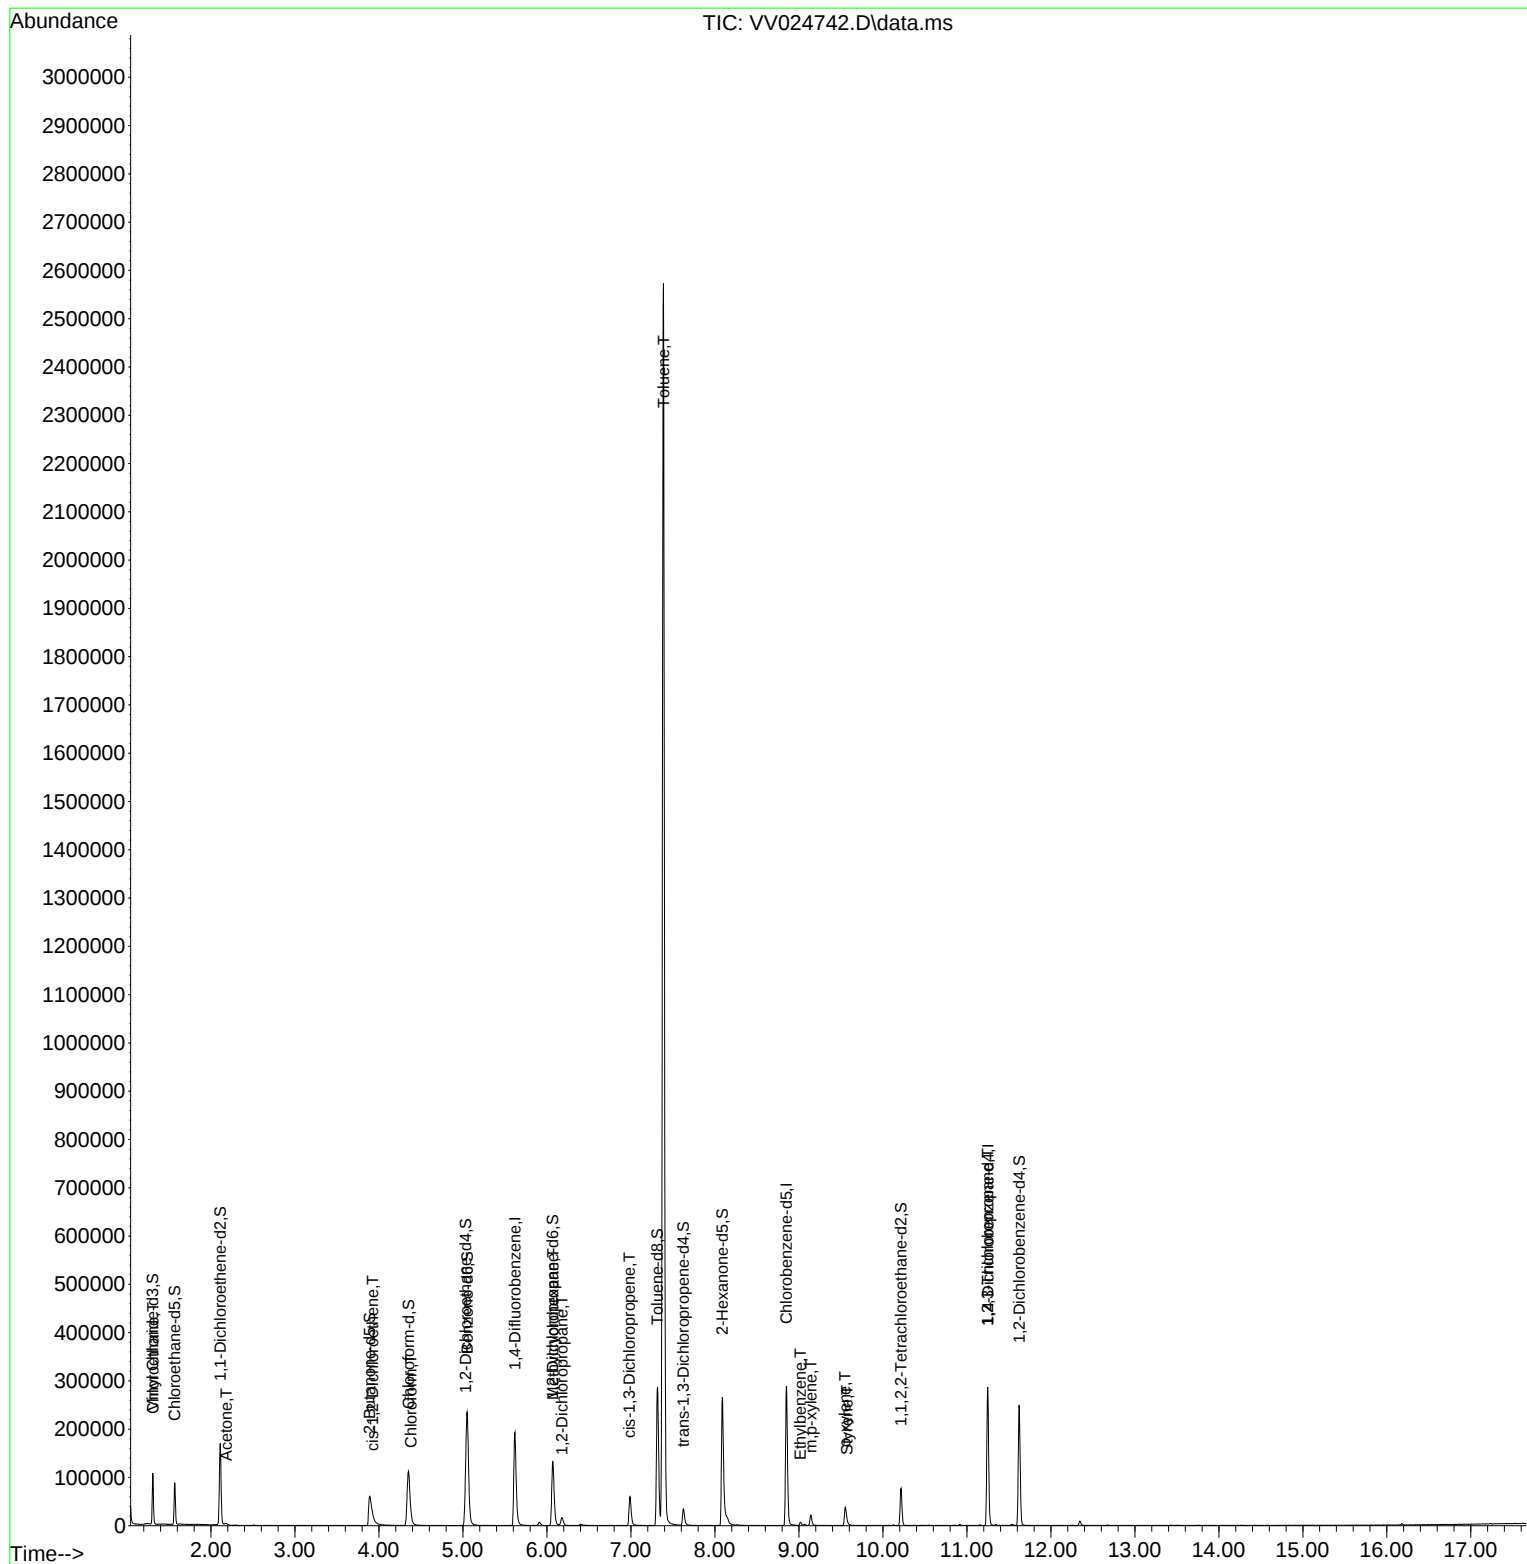


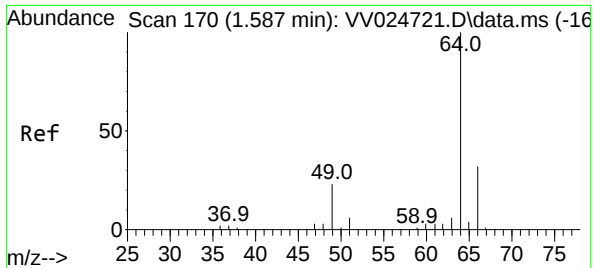

#8
Chloroethane
Concen: 0.087 ug/L
RT: 1.310 min Scan# 84
Delta R.T. -0.277 min
Lab File: VV024742.D
Acq: 17 Feb 2022 23:07




Instrument :
MSVOA_V
ClientSampleId :
F4M92


Tgt Ion: 64 Resp: 956
Ion Ratio Lower Upper
64 100
66 190.0 22.5 41.9#

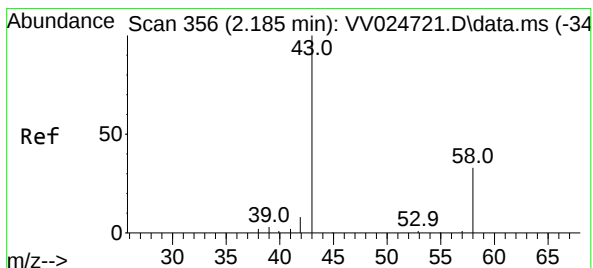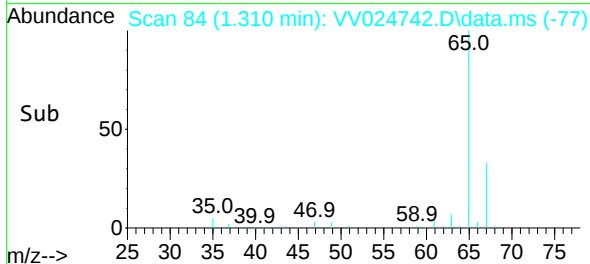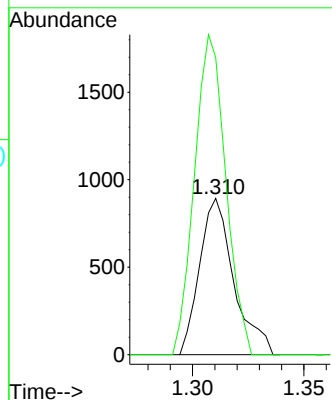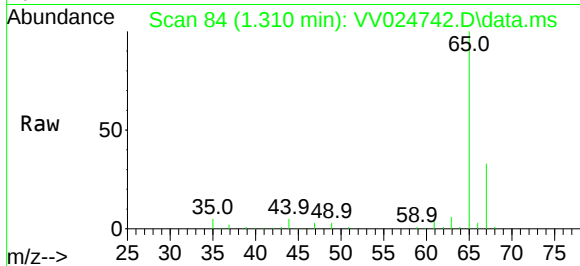

#13
Acetone
Concen: 4.024 ug/L
RT: 2.182 min Scan# 355
Delta R.T. -0.003 min
Lab File: VV024742.D
Acq: 17 Feb 2022 23:07

Tgt Ion: 43 Resp: 5744
Ion Ratio Lower Upper
43 100
58 30.9 0.0 63.6


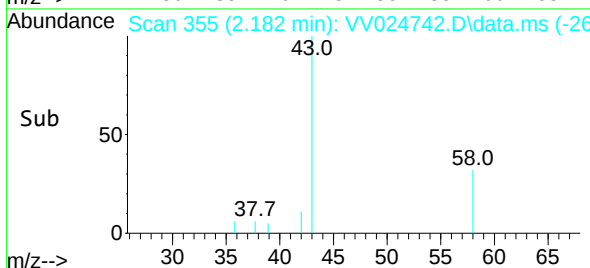
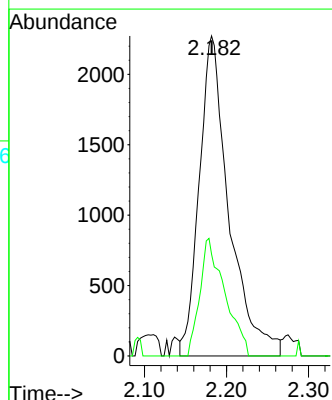
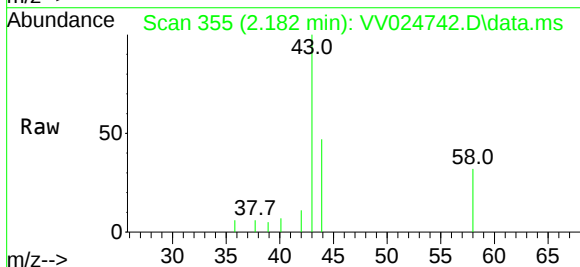


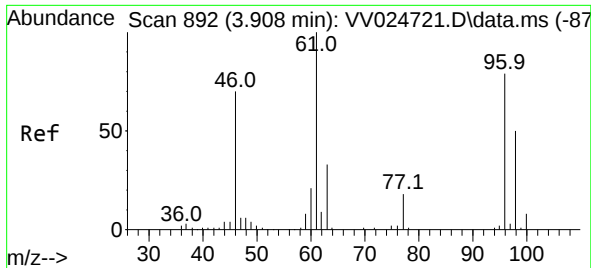

#22
 cis-1,2-Dichloroethene
 Concen: 0.094 ug/L
 RT: 3.924 min Scan# 89
 Delta R.T. 0.016 min
 Lab File: VV024742.D
 Acq: 17 Feb 2022 23:07




Instrument :
 MSVOA_V
 ClientSampleId :
 F4M92


Tgt Ion: 96 Resp: 1268
 Ion Ratio Lower Upper
 96 100
 61 98.3 89.7 166.5
 68 0.0 0.0 0.0

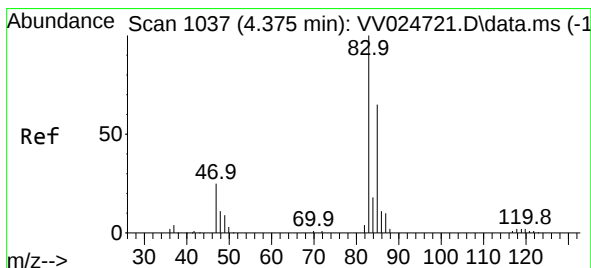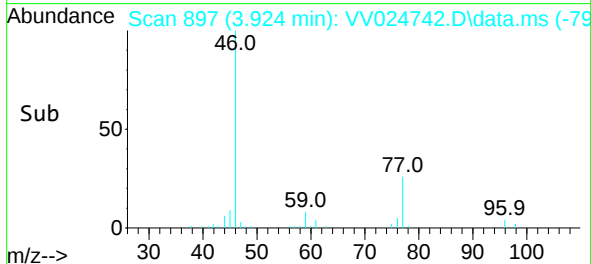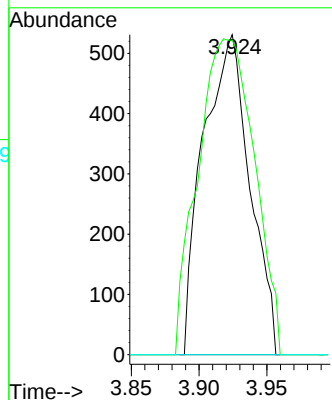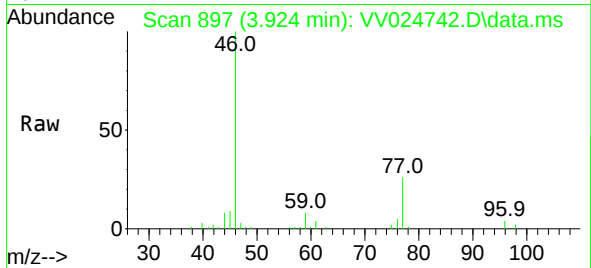

#25
 Chloroform
 Concen: 0.197 ug/L
 RT: 4.381 min Scan# 1039
 Delta R.T. 0.006 min
 Lab File: VV024742.D
 Acq: 17 Feb 2022 23:07

Tgt Ion: 83 Resp: 4791
 Ion Ratio Lower Upper
 83 100
 85 67.6 45.5 84.5

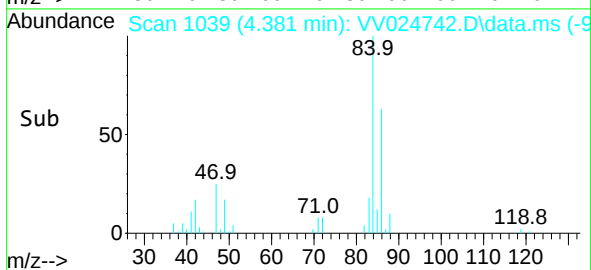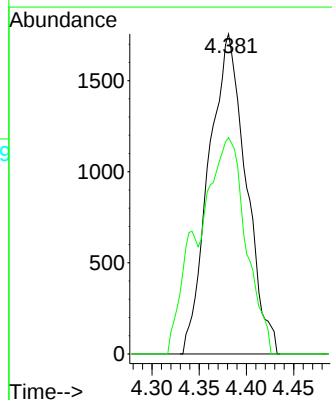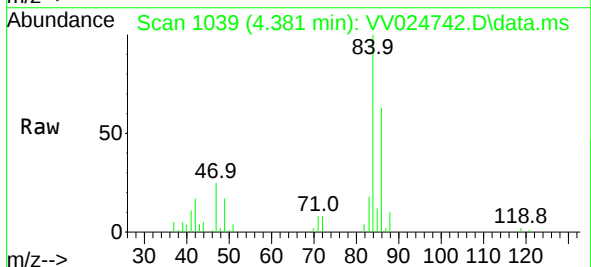

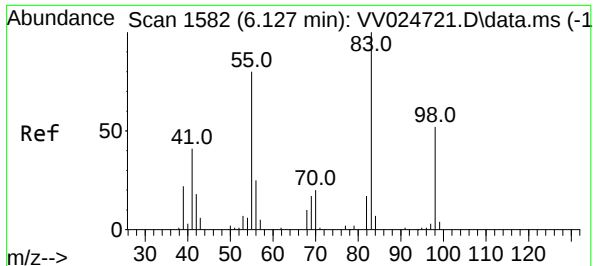

#35

Methylcyclohexane

Concen: 0.717 ug/L

RT: 6.072 min Scan# 11

Delta R.T. -0.055 min

Lab File: VV024742.D

Acq: 17 Feb 2022 23:07

Instrument :

MSVOA_V

ClientSampleId :

F4M92





Tgt Ion: 83 Resp: 16264

Ion Ratio Lower Upper

83 100

55 0.4 58.8 88.2#

98 0.7 38.6 58.0#

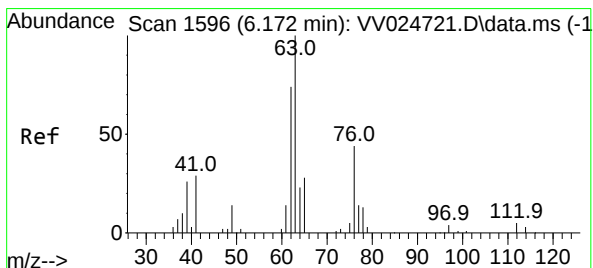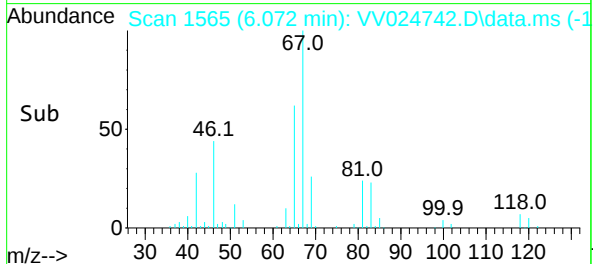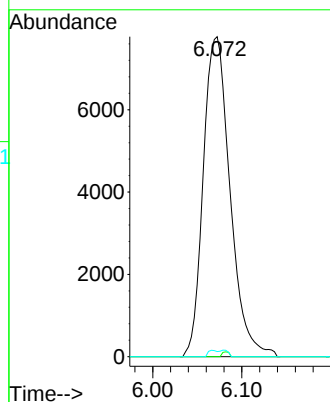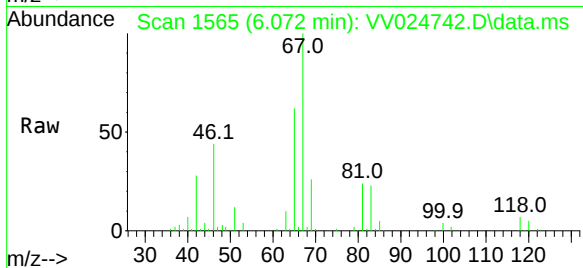

#37

1,2-Dichloropropane

Concen: 0.552 ug/L

RT: 6.178 min Scan# 1598

Delta R.T. 0.006 min

Lab File: VV024742.D




Acq: 17 Feb 2022 23:07


Tgt Ion: 63 Resp: 6916

Ion Ratio Lower Upper

63 100

112 1.1 3.8 5.6#

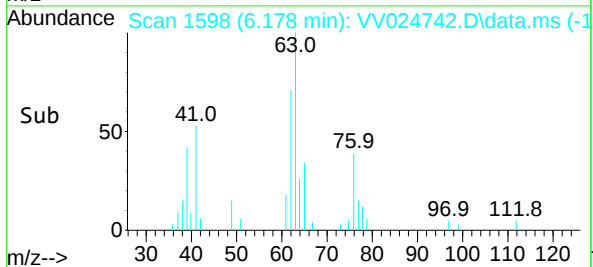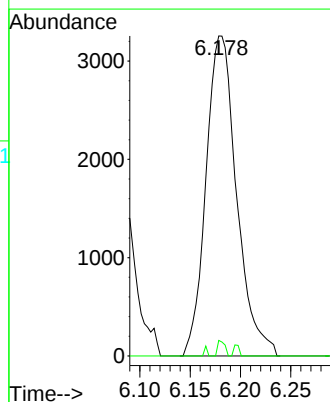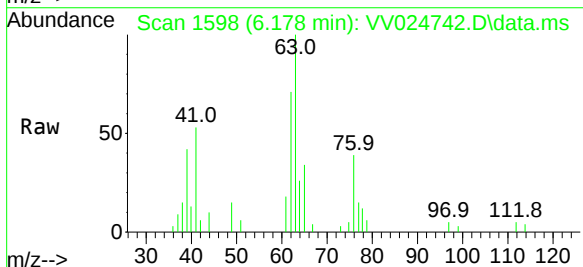

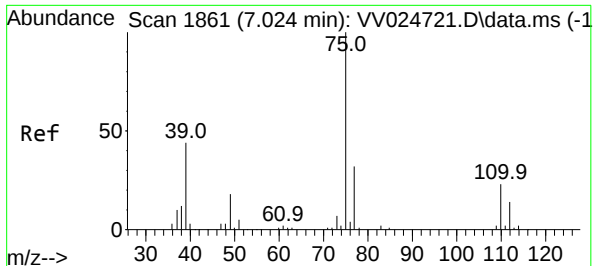

#39

cis-1,3-Dichloropropene

Concen: 0.086 ug/L

RT: 6.982 min Scan# 11

Delta R.T. -0.042 min

Lab File: VV024742.D

Acq: 17 Feb 2022 23:07

Instrument :

MSVOA_V

ClientSampleId :





F4M92

Tgt Ion: 75 Resp: 1494

Ion Ratio Lower Upper

75 100

77 46.8 22.3 41.5#

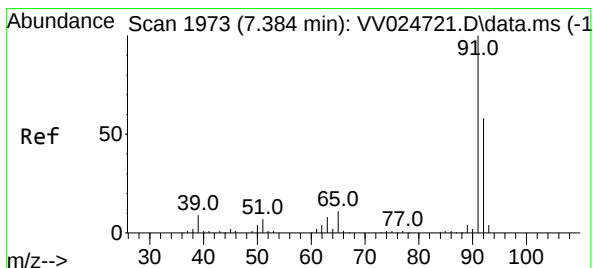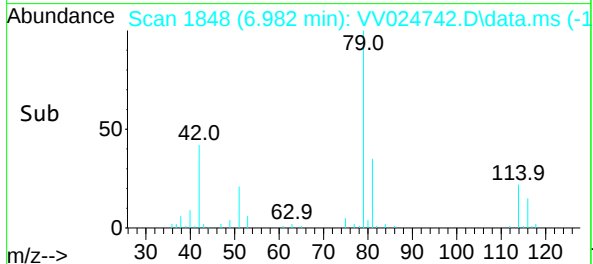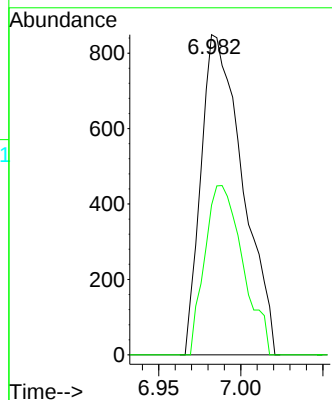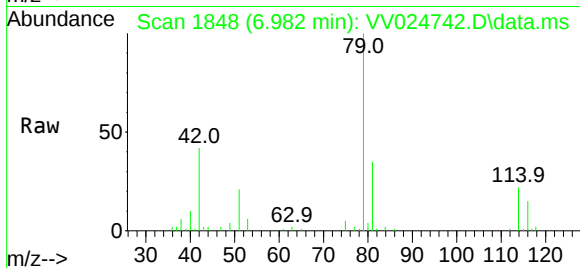

#42

Toluene

Concen: 32.358 ug/L

RT: 7.387 min Scan# 1974

Delta R.T. 0.003 min

Lab File: VV024742.D




Acq: 17 Feb 2022 23:07


Tgt Ion: 91 Resp: 1825767

Ion Ratio Lower Upper

91 100

92 59.0 40.3 74.9

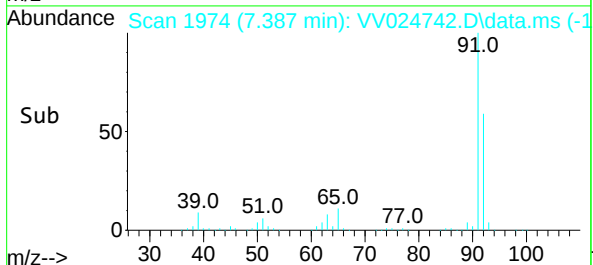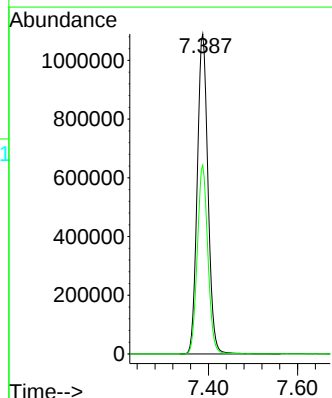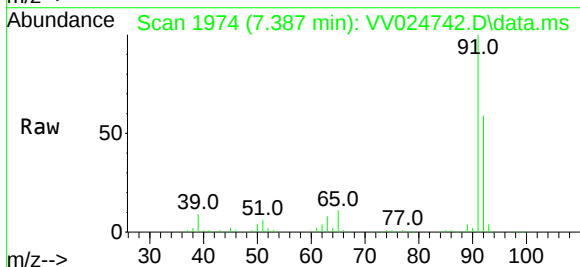

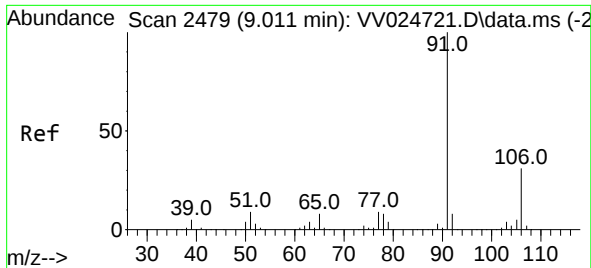

#52

Ethylbenzene

Concen: 0.083 ug/L

RT: 9.017 min Scan# 24

Delta R.T. 0.006 min

Lab File: VV024742.D

Acq: 17 Feb 2022 23:07

Instrument :

MSVOA_V

ClientSampleId :





F4M92

Tgt Ion: 91 Resp: 5104

Ion Ratio Lower Upper

91 100

106 31.4 21.3 39.5

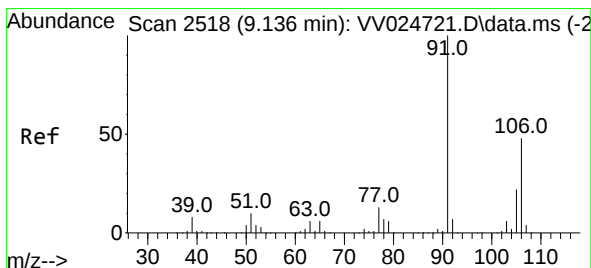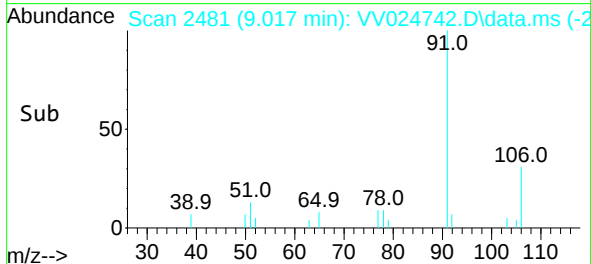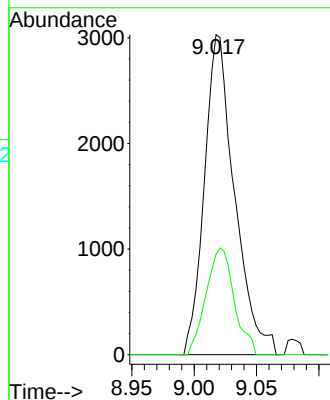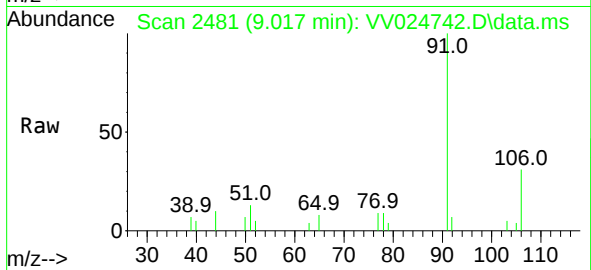

#53

m,p-xylene

Concen: 0.284 ug/L

RT: 9.143 min Scan# 2520

Delta R.T. 0.006 min

Lab File: VV024742.D




Acq: 17 Feb 2022 23:07


Tgt Ion:106 Resp: 6622

Ion Ratio Lower Upper

106 100

91 186.7 143.6 266.6


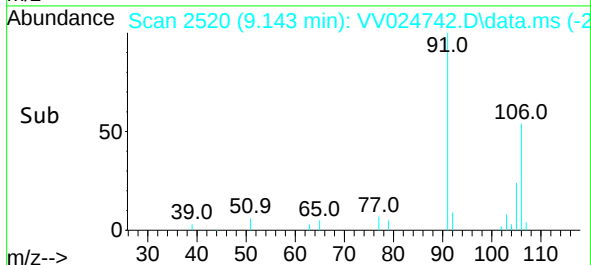
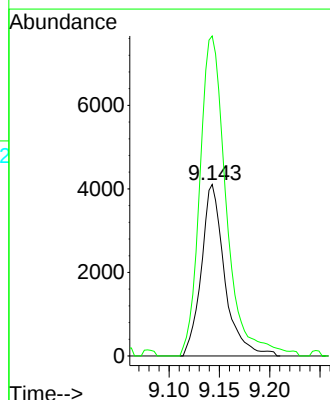
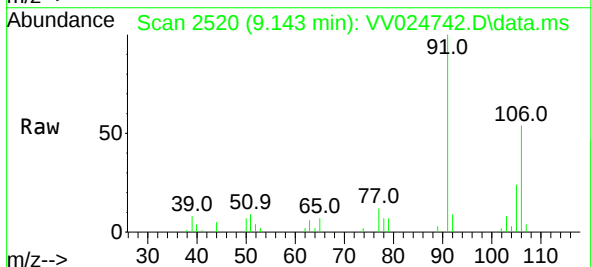


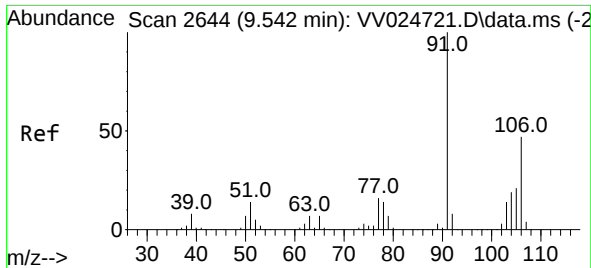

#54
o-xylene
Concen: 0.117 ug/L
RT: 9.548 min Scan# 2653
Delta R.T. 0.006 min
Lab File: VV024742.D
Acq: 17 Feb 2022 23:07




Instrument :
MSVOA_V
ClientSampleId :
F4M92


Tgt Ion:106 Resp: 2661
Ion Ratio Lower Upper
106 100
91 218.3 152.2 282.7

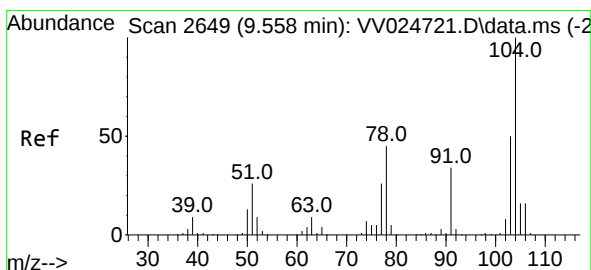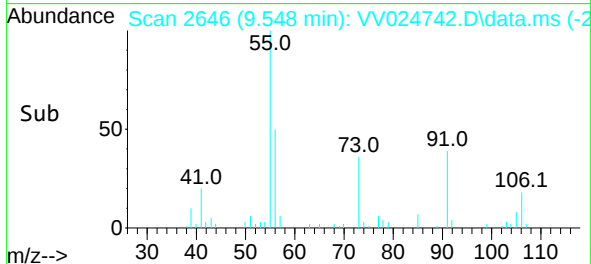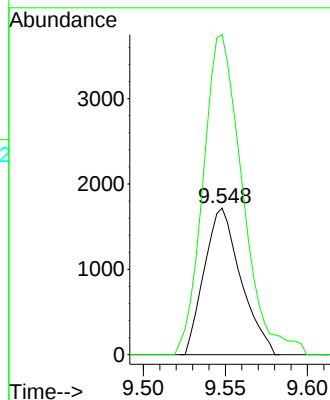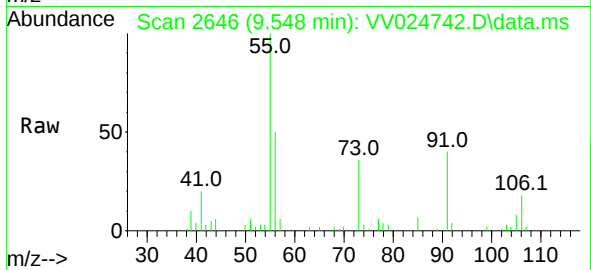

#55
Styrene
Concen: 0.076 ug/L
RT: 9.570 min Scan# 2653
Delta R.T. 0.013 min
Lab File: VV024742.D
Acq: 17 Feb 2022 23:07

Tgt Ion:104 Resp: 2798
Ion Ratio Lower Upper
104 100
78 44.4 32.0 59.4

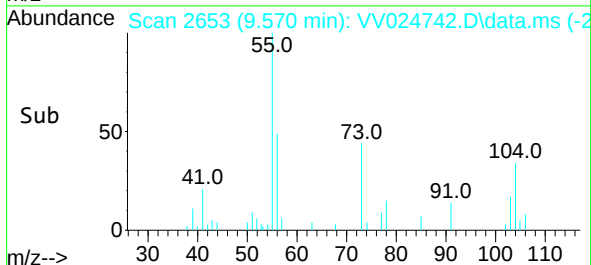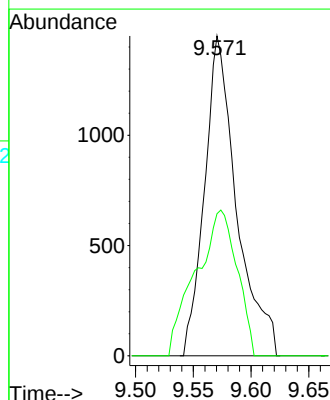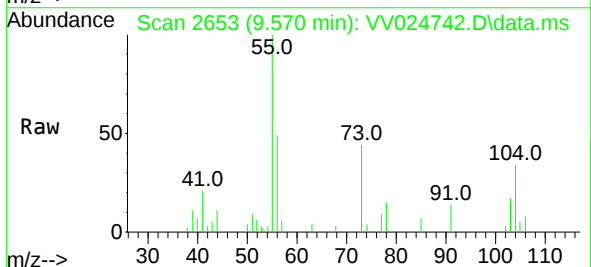

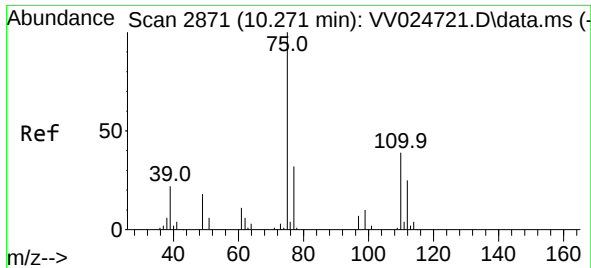

#61

1,2,3-Trichloropropane

Concen: 1.445 ug/L

RT: 11.246 min Scan# 31

Delta R.T. 0.974 min

Lab File: VV024742.D


Acq: 17 Feb 2022 23:07

Instrument :

MSVOA_V

ClientSampleId :

F4M92

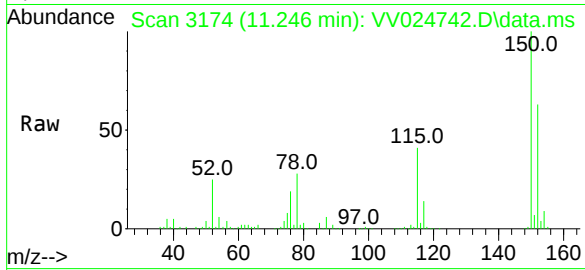

Tgt Ion: 75 Resp: 9121

Ion Ratio Lower Upper

75 100

77 32.5 26.3 39.5

110 2.1 30.3 45.5#

