

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW021722\
 Data File : VW024727.D
 Acq On : 17 Feb 2022 17:14
 Operator : SY/MD
 Sample : N1510-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4M25

Quant Time: Feb 18 07:34:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Feb 18 07:32:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	170249	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	158015	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	70292	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	67394	4.667	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	93.400%	
7) Chloroethane-d5	1.568	69	55820	4.712	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	94.200%	
11) 1,1-Dichloroethene-d2	2.111	63	89878	3.396	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	68.000%	
20) 2-Butanone-d5	3.889	46	105990	51.386	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	102.780%	
24) Chloroform-d	4.352	84	101665	4.512	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	90.200%	
26) 1,2-Dichloroethane-d4	5.034	65	48598	4.839	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	96.800%	
32) Benzene-d6	5.050	84	216269	4.744	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	94.800%	
36) 1,2-Dichloropropane-d6	6.069	67	64817	4.832	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	96.600%	
41) Toluene-d8	7.317	98	191182	4.616	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	92.400%	
43) trans-1,3-Dichloroprop...	7.625	79	20057	4.488	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	89.800%	
46) 2-Hexanone-d5	8.088	63	83433	47.445	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	94.900%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	38178	4.722	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	94.400%	
66) 1,2-Dichlorobenzene-d4	11.622	152	58762	4.831	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	96.600%	
Target Compounds					Qvalue	
25) Chloroform	4.378	83	2912	0.118	ug/L	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021722\
Data File : VV024727.D
Acq On : 17 Feb 2022 17:14
Operator : SY/MD
Sample : N1510-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4M25

Quant Time: Feb 18 07:34:44 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Feb 18 07:32:51 2022
Response via : Initial Calibration

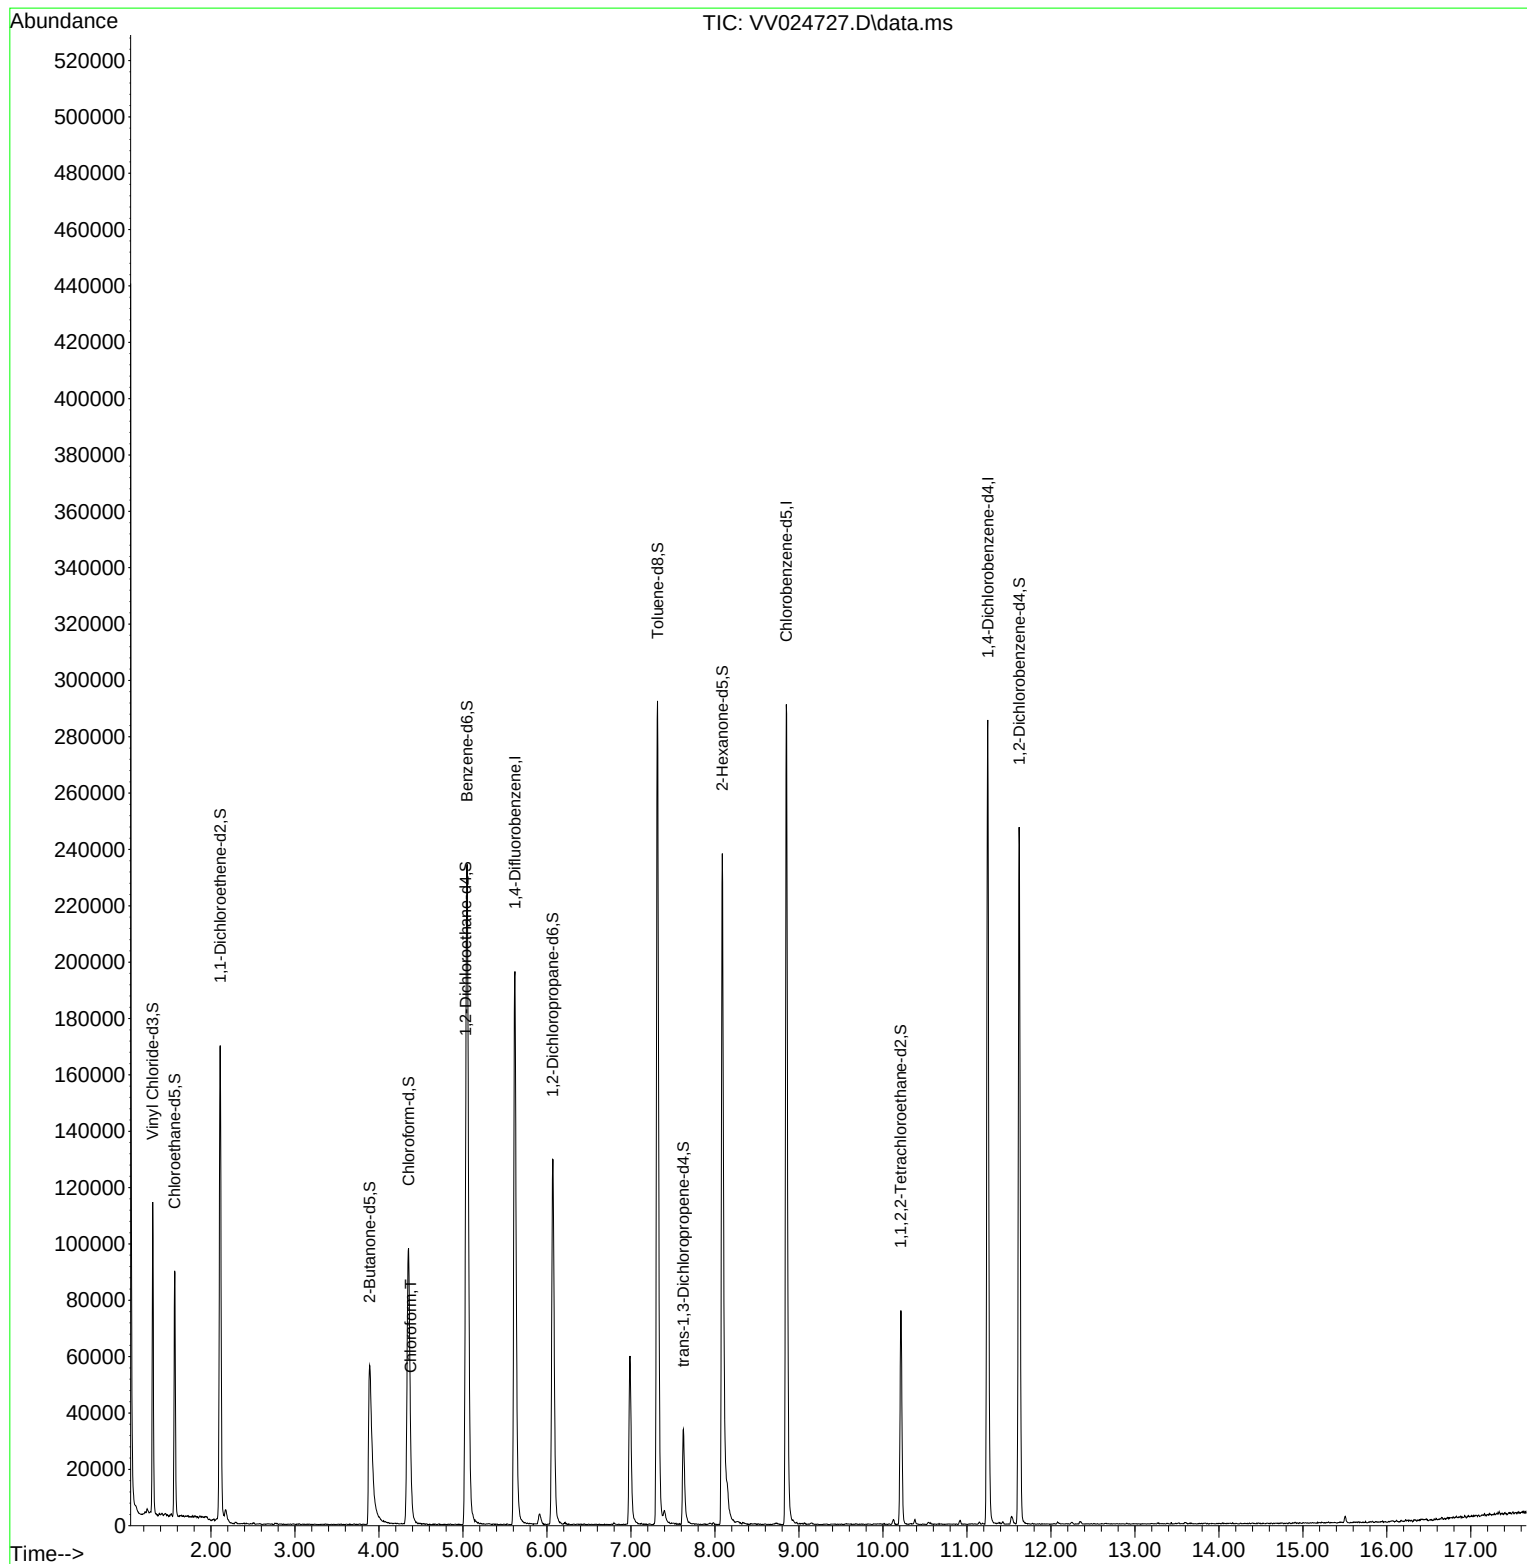

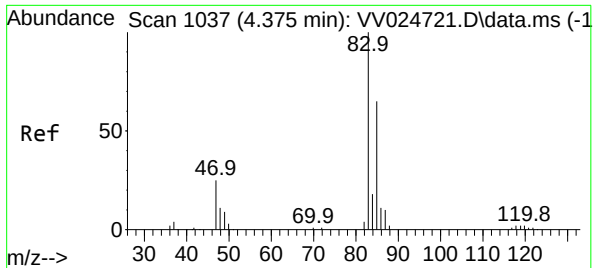

#25

Chloroform

Concen: 0.118 ug/L

RT: 4.378 min Scan# 10

Delta R.T. 0.003 min

Lab File: VV024727.D


Acq: 17 Feb 2022 17:14

Instrument :

MSVOA_V

ClientSampleId :

F4M25

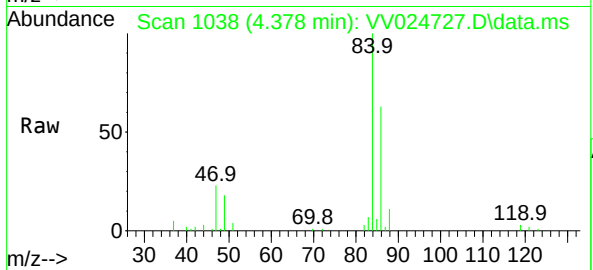

Tgt Ion: 83 Resp: 2912

Ion Ratio Lower Upper

83 100

85 76.4 45.5 84.5

