

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW021722\
 Data File : VW024729.D
 Acq On : 17 Feb 2022 18:01
 Operator : SY/MD
 Sample : N1510-09RE
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4M30

Quant Time: Feb 18 07:35:14 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Feb 18 07:32:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	71295	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	65265	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	28084	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	29622	4.898	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	98.000%	
7) Chloroethane-d5	1.568	69	24636	4.966	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	99.400%	
11) 1,1-Dichloroethene-d2	2.111	63	40910	3.692	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	73.800%	
20) 2-Butanone-d5	3.883	46	77285	89.475	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	178.940%#	
24) Chloroform-d	4.352	84	44455	4.711	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	94.200%	
26) 1,2-Dichloroethane-d4	5.037	65	26717	6.352	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	127.000%	
32) Benzene-d6	5.053	84	92835	4.931	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	98.600%	
36) 1,2-Dichloropropane-d6	6.072	67	29519	5.328	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	106.600%	
41) Toluene-d8	7.317	98	80843	4.725	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	94.600%	
43) trans-1,3-Dichloroprop...	7.628	79	10548	5.714	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	114.200%	
46) 2-Hexanone-d5	8.088	63	57107	78.626	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	157.260%#	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	24381	7.301	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	146.000%#	
66) 1,2-Dichlorobenzene-d4	11.625	152	26755	5.506	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	110.200%	
Target Compounds					Qvalue	
13) Acetone	2.169	43	2777	4.559	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021722\
Data File : VV024729.D
Acq On : 17 Feb 2022 18:01
Operator : SY/MD
Sample : N1510-09RE
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4M30

Quant Time: Feb 18 07:35:14 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Feb 18 07:32:51 2022
Response via : Initial Calibration

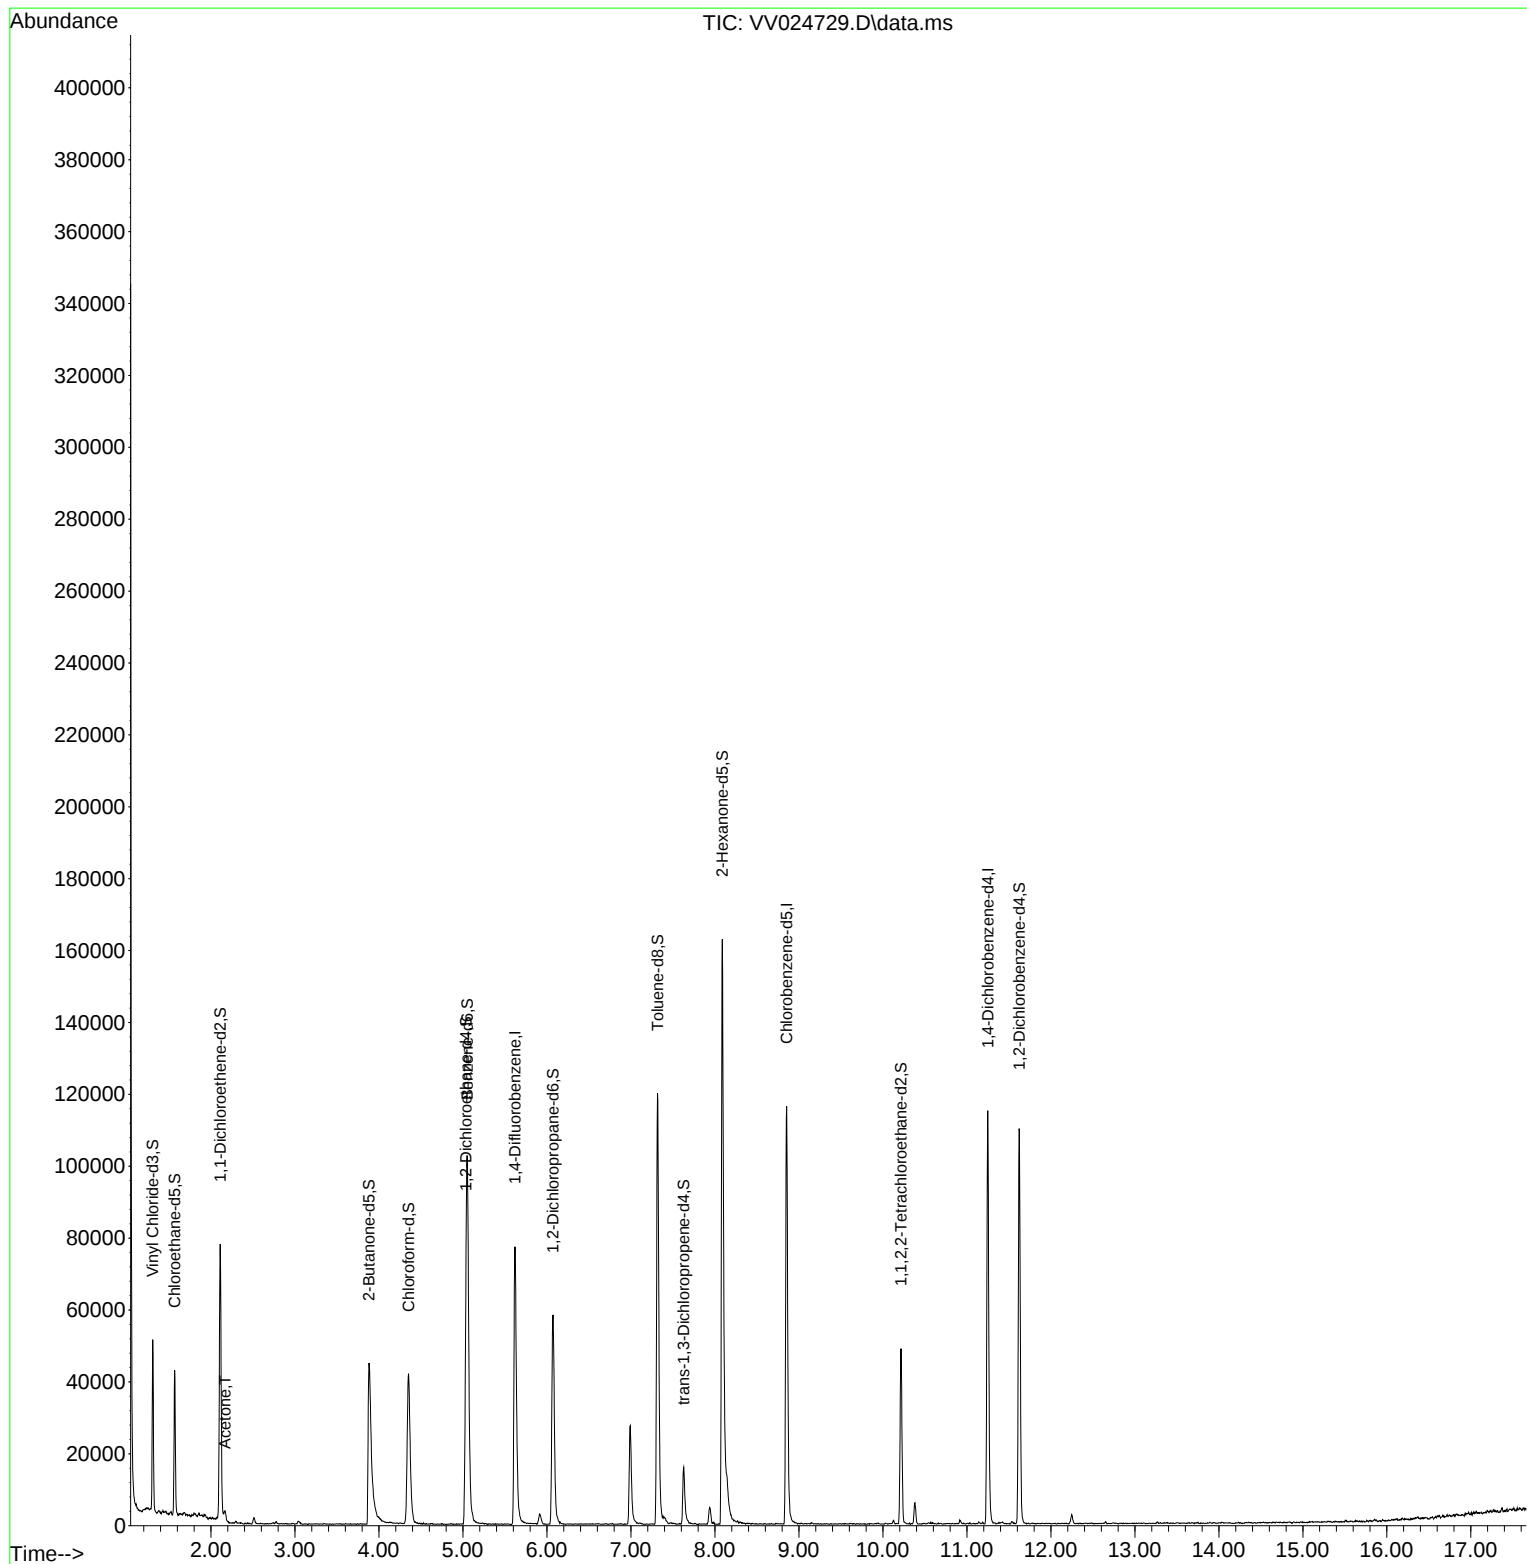

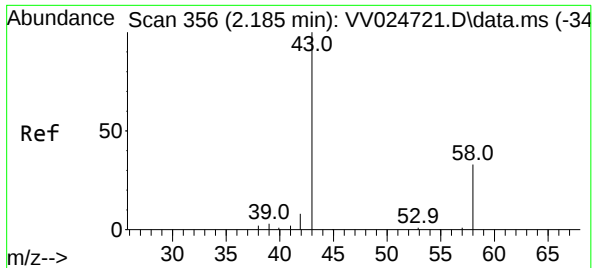

#13
 Acetone
 Concen: 4.559 ug/L
 RT: 2.169 min Scan# 31
 Delta R.T. -0.016 min
 Lab File: VV024729.D
 Acq: 17 Feb 2022 18:01

Instrument :
 MSVOA_V
 ClientSampleId :
 F4M30

Tgt Ion: 43 Resp: 2777
 Ion Ratio Lower Upper
 43 100
 58 29.9 0.0 63.6

