

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW021722\
 Data File : VW024738.D
 Acq On : 17 Feb 2022 21:33
 Operator : SY/MD
 Sample : N1510-19
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4M28

Quant Time: Feb 18 07:37:20 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Feb 18 07:32:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	164410	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	152224	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	68347	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	64858	4.651	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	93.000%
7) Chloroethane-d5	1.568	69	54102	4.729	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	94.600%
11) 1,1-Dichloroethene-d2	2.108	63	87004	3.405	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	68.000%
20) 2-Butanone-d5	3.889	46	112631	56.545	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	113.080%
24) Chloroform-d	4.349	84	99112	4.555	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.000%
26) 1,2-Dichloroethane-d4	5.034	65	48963	5.048	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.000%
32) Benzene-d6	5.050	84	210655	4.797	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.000%
36) 1,2-Dichloropropane-d6	6.069	67	63545	4.917	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.400%
41) Toluene-d8	7.317	98	188299	4.719	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.400%
43) trans-1,3-Dichloroprop...	7.625	79	20403	4.739	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	94.800%
46) 2-Hexanone-d5	8.088	63	92725	54.735	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	109.480%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	40250	5.168	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	103.400%
66) 1,2-Dichlorobenzene-d4	11.622	152	58455	4.943	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.800%
Target Compounds						
					Qvalue	
25) Chloroform	4.372	83	3172	0.133	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021722\
Data File : VV024738.D
Acq On : 17 Feb 2022 21:33
Operator : SY/MD
Sample : N1510-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4M28

Quant Time: Feb 18 07:37:20 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Feb 18 07:32:51 2022
Response via : Initial Calibration

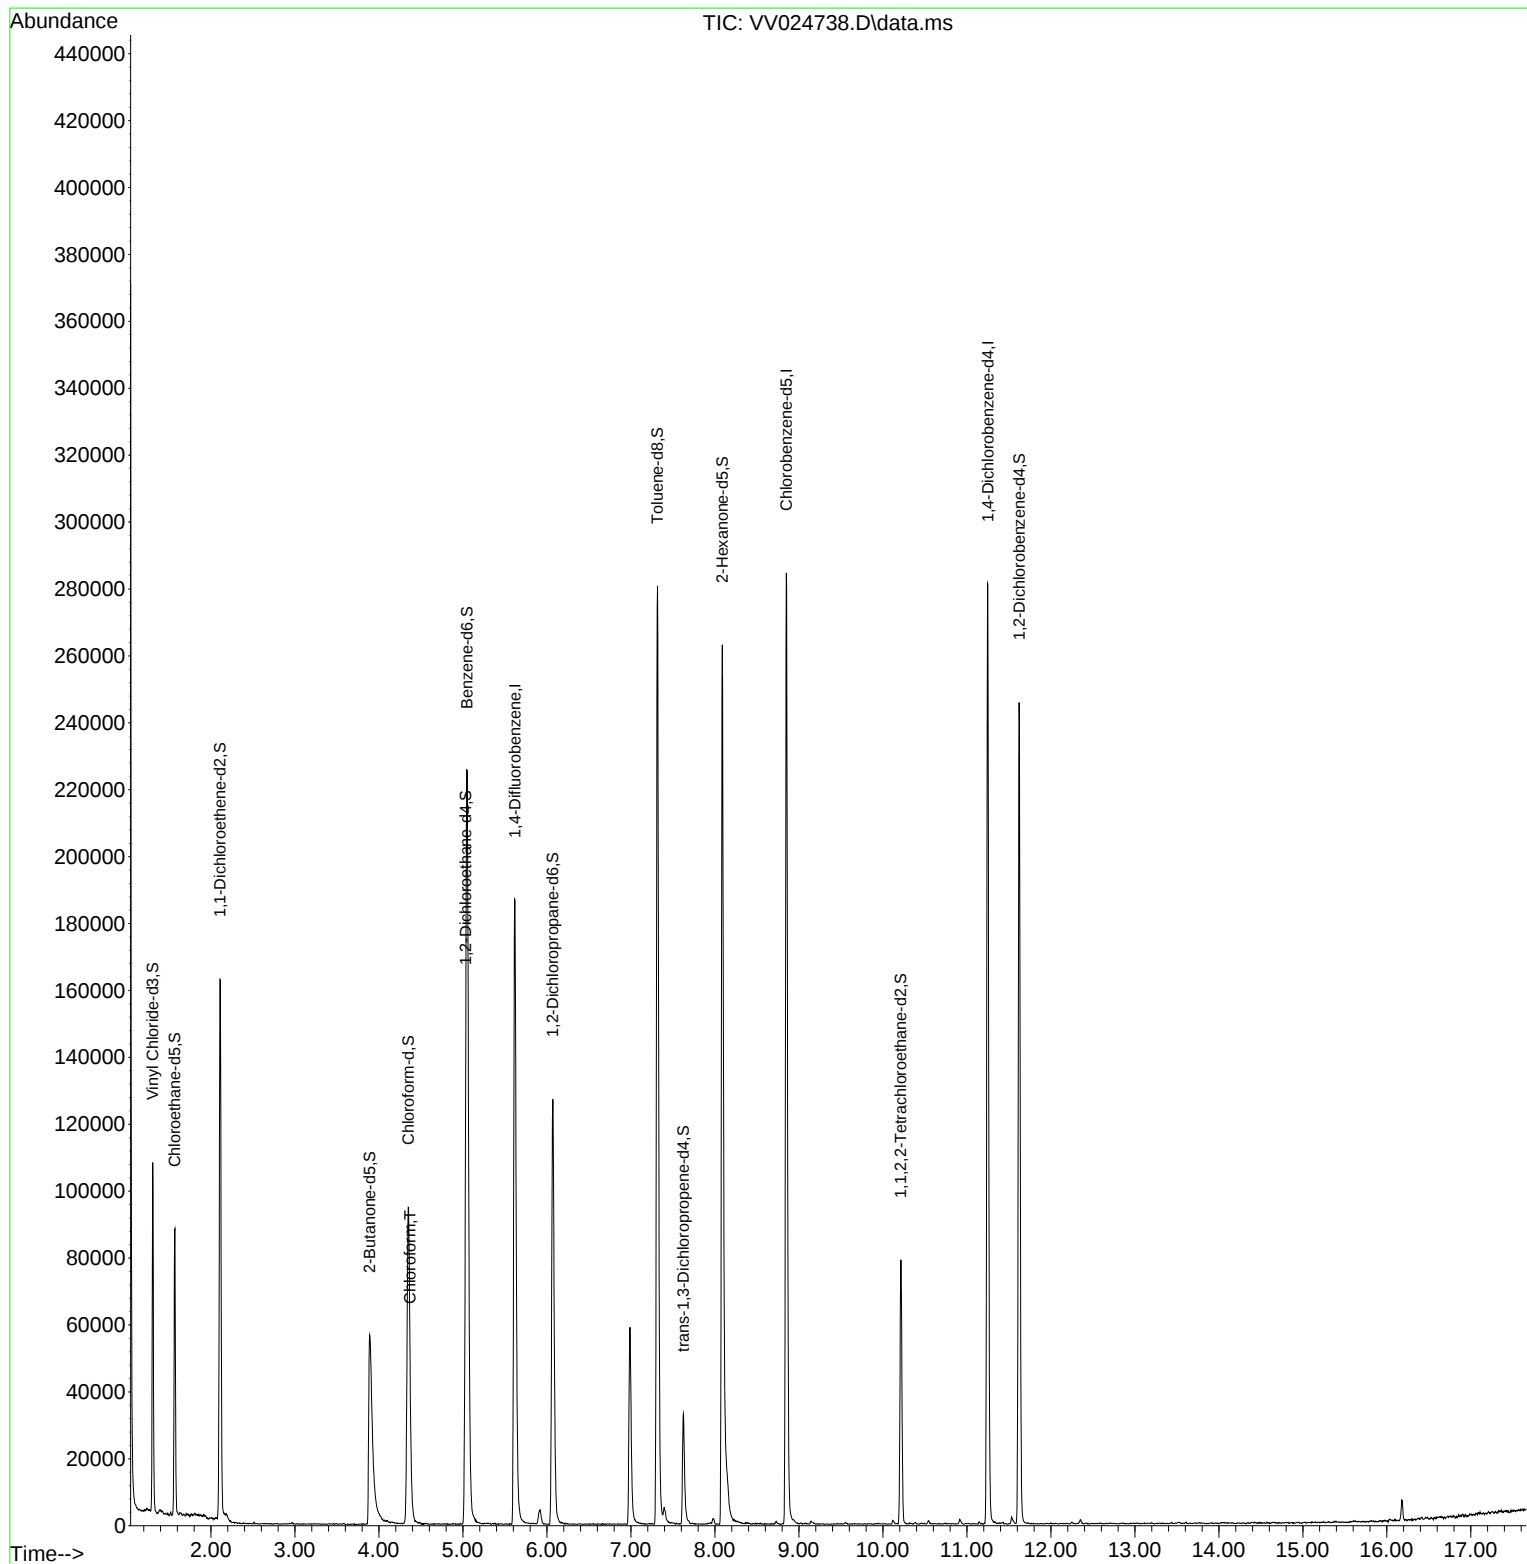

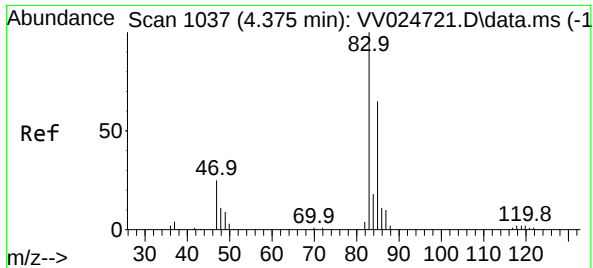

#25
 Chloroform
 Concen: 0.133 ug/L
 RT: 4.372 min Scan# 10
 Delta R.T. -0.003 min
 Lab File: VV024738.D
 Acq: 17 Feb 2022 21:33

Instrument :
 MSVOA_V
 ClientSampleId :
 F4M28

Tgt Ion: 83 Resp: 3172
 Ion Ratio Lower Upper
 83 100
 85 60.3 45.5 84.5

