

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021722\
 Data File : VV024722.D
 Acq On : 17 Feb 2022 15:17
 Operator : SY/MD
 Sample : VV0217WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK307

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV024722.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	95	rVB	119346	118070	19.01%	2.397%
2	1.568	157	164	179	rVB	94819	106536	17.15%	2.162%
3	2.108	322	332	359	rVB	184533	271775	43.76%	5.517%
4	2.513	448	458	466	rBV2	4277	6709	1.08%	0.136%
5	3.895	878	888	929	rBV	52117	171875	27.67%	3.489%
6	4.352	1010	1030	1056	rBV2	103247	264557	42.59%	5.370%
7	5.050	1230	1247	1283	rBV2	251031	621115	100.00%	12.607%
8	5.619	1412	1424	1453	rBV	197699	399772	64.36%	8.115%
9	5.911	1506	1515	1530	rVB6	4300	9737	1.57%	0.198%
10	6.069	1544	1564	1593	rBV2	137883	286709	46.16%	5.820%
11	6.989	1837	1850	1881	rBV	67893	124918	20.11%	2.536%
12	7.317	1937	1952	1970	rBV	314037	549348	88.45%	11.151%
13	7.400	1972	1978	1993	rVB3	4541	9201	1.48%	0.187%
14	7.625	2038	2048	2073	rBV	35975	64613	10.40%	1.312%
15	8.088	2182	2192	2234	rBV	248428	470996	75.83%	9.560%
16	8.850	2416	2429	2453	rBV	285382	476796	76.76%	9.678%
17	10.217	2842	2854	2871	rBV	79206	125634	20.23%	2.550%
18	11.249	3163	3175	3196	rBV	283081	439545	70.77%	8.922%
19	11.622	3280	3291	3313	rBV	262038	408664	65.80%	8.295%




Sum of corrected areas: 4926570

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021722\
Data File : VV024722.D
Acq On : 17 Feb 2022 15:17
Operator : SY/MD
Sample : VV0217WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK307

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

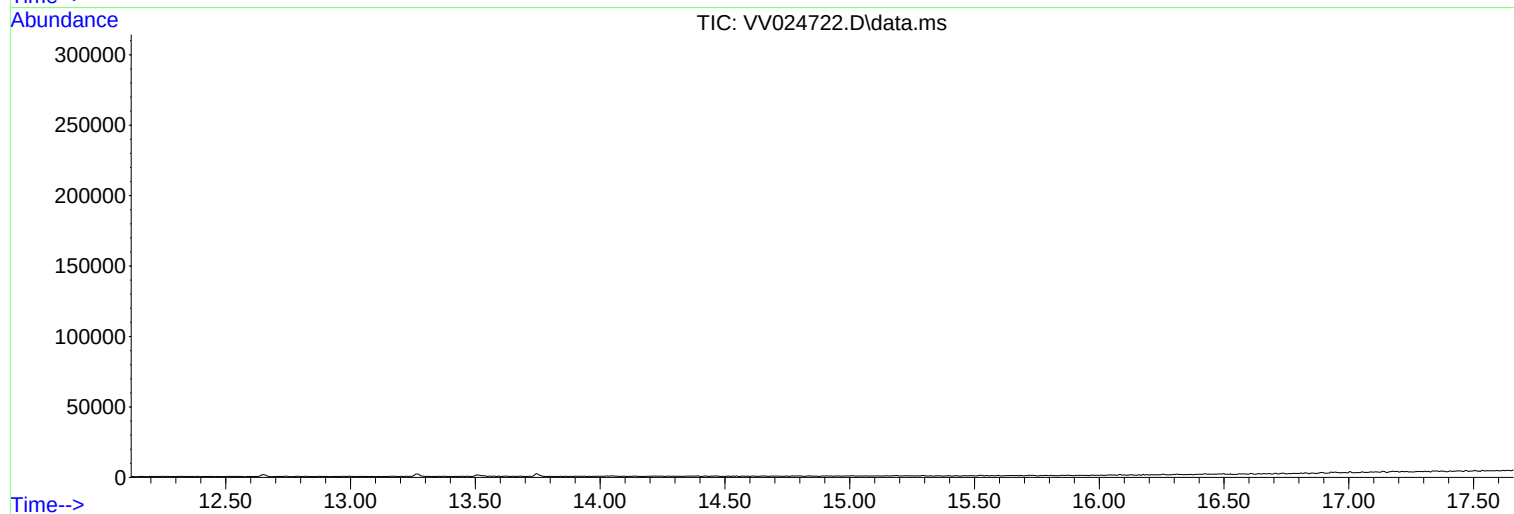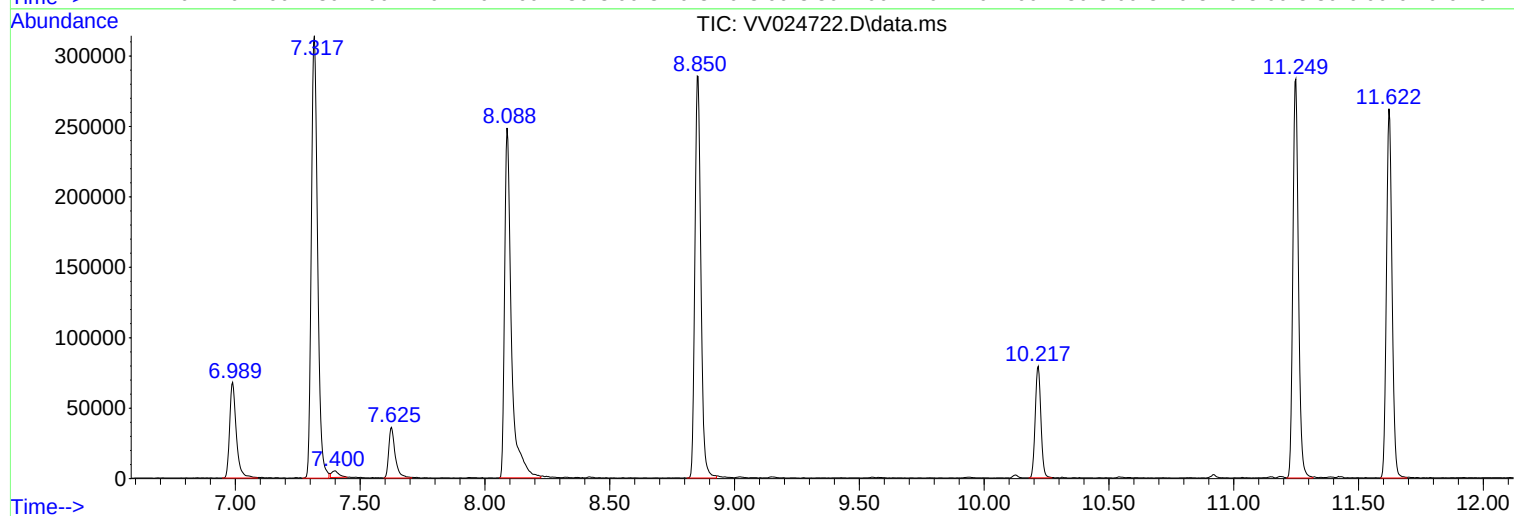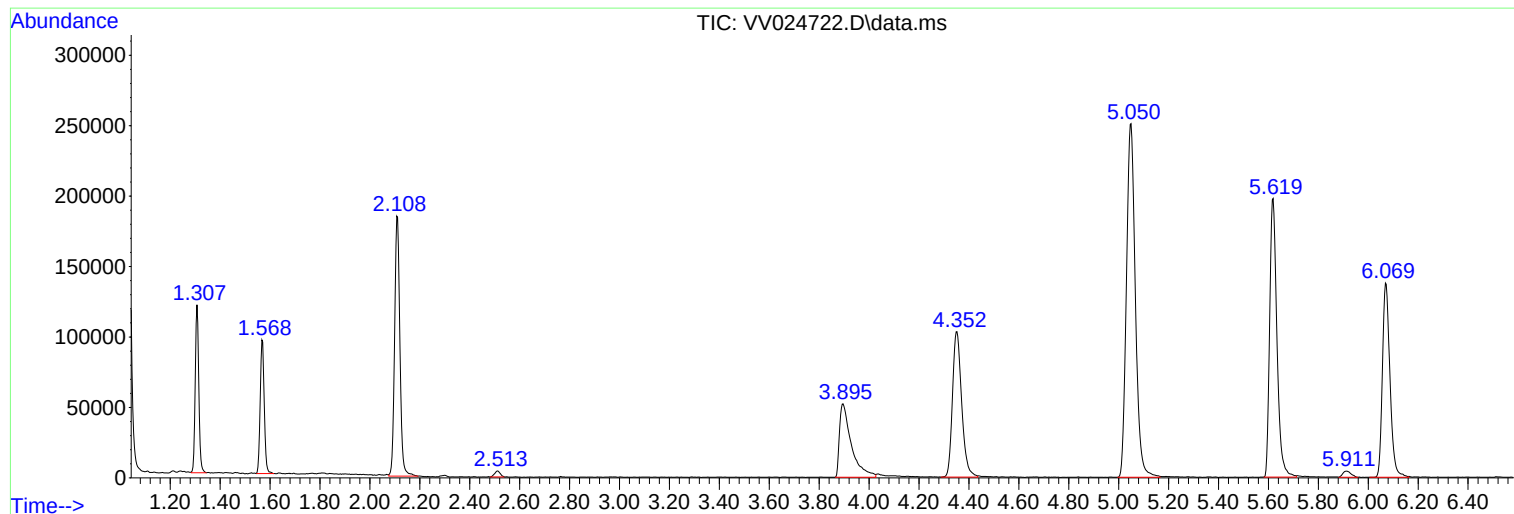

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021722\
Data File : VV024722.D
Acq On : 17 Feb 2022 15:17
Operator : SY/MD
Sample : VV0217WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK307

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021722\
Data File : VV024722.D
Acq On : 17 Feb 2022 15:17
Operator : SY/MD
Sample : VV0217WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK307

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc