

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021722\
 Data File : VV024729.D
 Acq On : 17 Feb 2022 18:01
 Operator : SY/MD
 Sample : N1510-09RE
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4M30

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV024729.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	98	rVB	48344	49566	15.56%	2.208%
2	1.568	157	164	176	rVB	40213	44059	13.83%	1.962%
3	2.111	323	333	344	rBV	76268	111462	35.00%	4.964%
4	3.883	876	884	916	rBV	44822	124796	39.18%	5.558%
5	4.352	1013	1030	1052	rBV	41700	104988	32.96%	4.676%
6	5.050	1232	1247	1272	rBV3	102570	261801	82.20%	11.660%
7	5.619	1411	1424	1451	rBV	77392	162467	51.01%	7.236%
8	5.911	1507	1515	1531	rVB7	2913	5920	1.86%	0.264%
9	6.072	1552	1565	1589	rBV2	58221	122105	38.34%	5.438%
10	6.992	1836	1851	1874	rBV	27403	52172	16.38%	2.324%
11	7.317	1941	1952	1970	rBV	119890	210820	66.19%	9.389%
12	7.628	2039	2049	2068	rBV2	15751	29397	9.23%	1.309%
13	7.937	2136	2145	2154	rBV2	4615	8171	2.57%	0.364%
14	8.088	2182	2192	2230	rBV	162737	318488	100.00%	14.185%
15	8.853	2420	2430	2455	rBV	116233	196853	61.81%	8.767%
16	10.217	2843	2854	2865	rBV	48733	75687	23.76%	3.371%
17	10.381	2895	2905	2920	rVB3	5960	9117	2.86%	0.406%
18	11.249	3164	3175	3194	rBV	114935	178279	55.98%	7.940%
19	11.622	3278	3291	3311	rBV	109913	174860	54.90%	7.788%
20	12.249	3475	3486	3500	rBV	2589	4301	1.35%	0.192%




Sum of corrected areas: 2245309

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021722\
Data File : VV024729.D
Acq On : 17 Feb 2022 18:01
Operator : SY/MD
Sample : N1510-09RE
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4M30

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

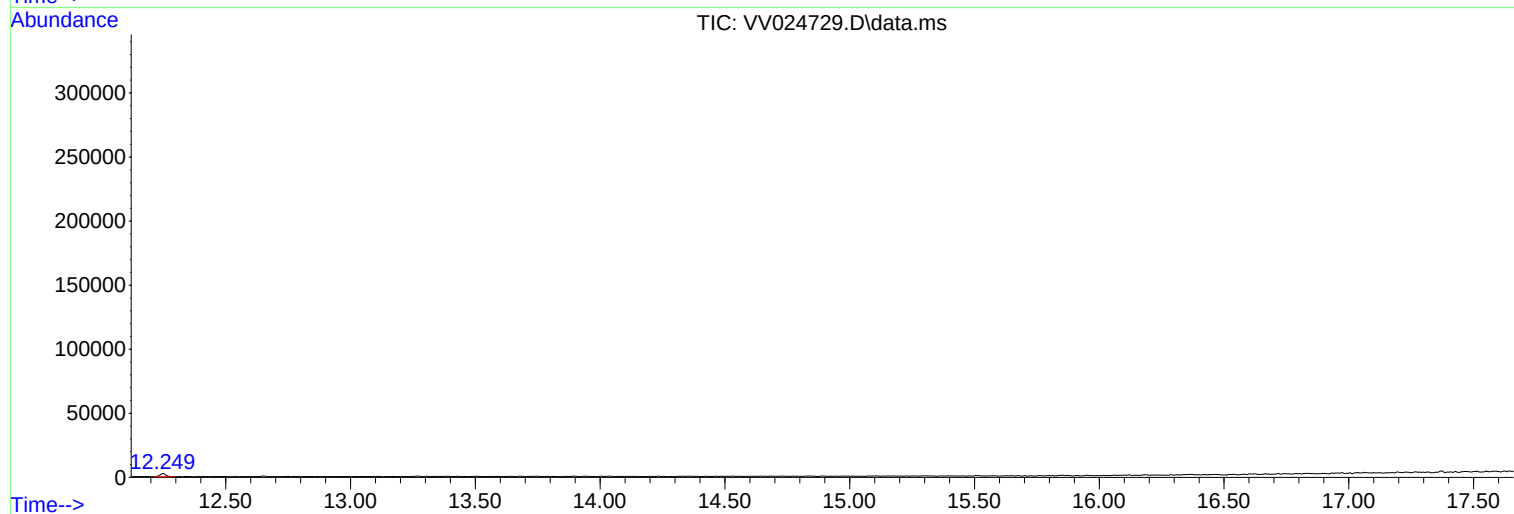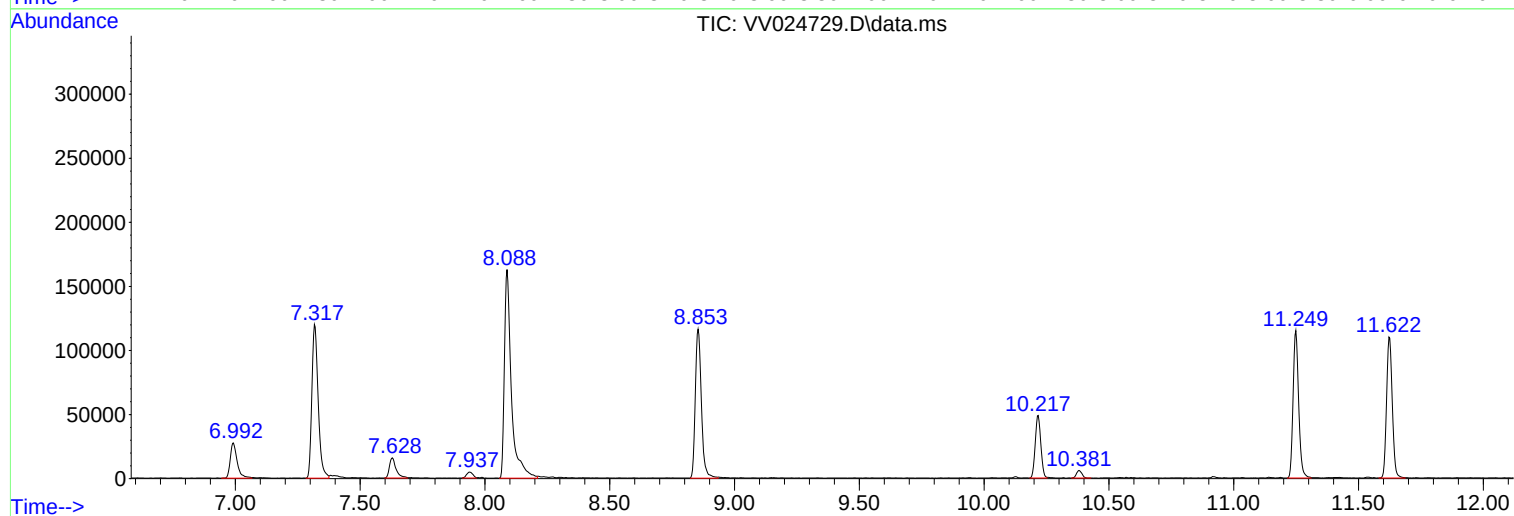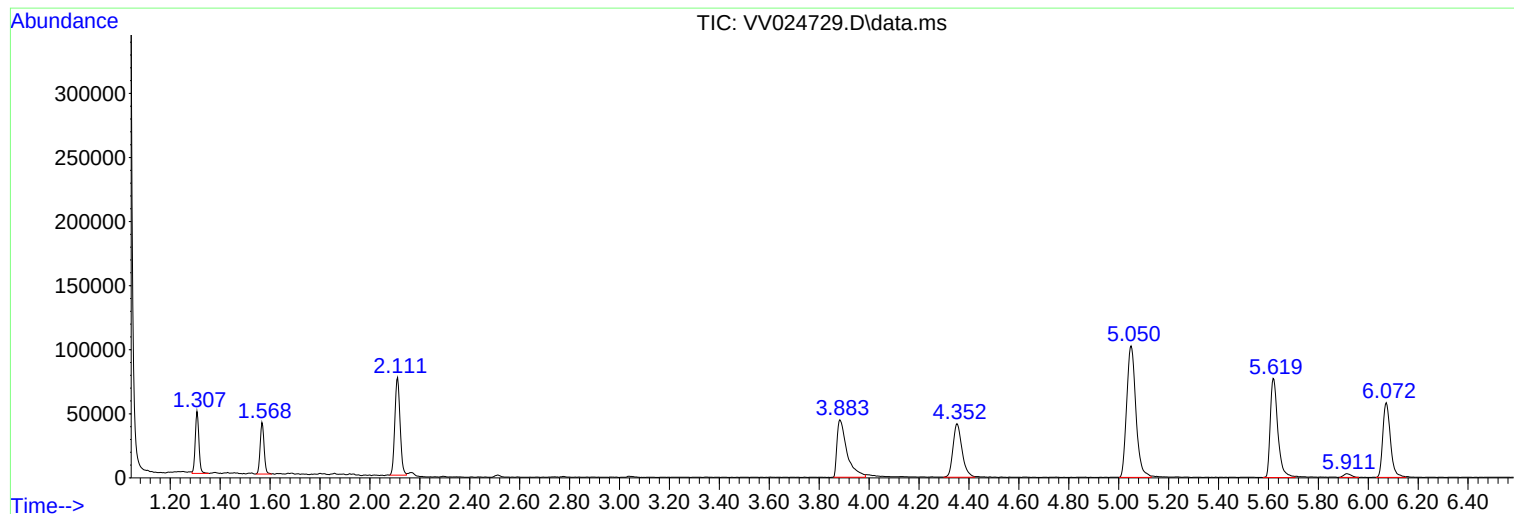

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021722\
Data File : VV024729.D
Acq On : 17 Feb 2022 18:01
Operator : SY/MD
Sample : N1510-09RE
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4M30

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021722\
Data File : VV024729.D
Acq On : 17 Feb 2022 18:01
Operator : SY/MD
Sample : N1510-09RE
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4M30

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
