

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021722\
 Data File : VV024740.D
 Acq On : 17 Feb 2022 22:20
 Operator : SY/MD
 Sample : N1522-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4M72

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV024740.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	96	rVB	109471	109464	19.03%	2.271%
2	1.568	156	164	177	rBV	87561	98809	17.18%	2.050%
3	2.111	322	333	351	rBV	164077	241811	42.04%	5.016%
4	2.574	473	477	488	rVB	15223	10166	1.77%	0.211%
5	3.895	877	888	921	rBV2	62495	223772	38.90%	4.642%
6	4.349	1009	1029	1058	rBV	111010	285744	49.68%	5.927%
7	5.047	1228	1246	1275	rBV2	233055	575207	100.00%	11.932%
8	5.619	1412	1424	1448	rBV	190077	386114	67.13%	8.009%
9	5.908	1505	1514	1528	rBV4	5591	11618	2.02%	0.241%
10	6.069	1552	1564	1586	rBV	127693	265912	46.23%	5.516%
11	6.989	1839	1850	1871	rBV	59499	110807	19.26%	2.298%
12	7.317	1938	1952	1969	rBV	288726	497027	86.41%	10.310%
13	7.394	1969	1976	1996	rVB	15762	31169	5.42%	0.647%
14	7.625	2037	2048	2069	rBV	32413	59359	10.32%	1.231%
15	8.088	2182	2192	2241	rVV	254986	495104	86.07%	10.270%
16	8.850	2417	2429	2460	rBV	284415	472194	82.09%	9.795%
17	10.217	2842	2854	2869	rBV	77142	121960	21.20%	2.530%
18	11.249	3164	3175	3197	rBV	283311	429838	74.73%	8.916%
19	11.554	3257	3270	3281	rBV5	5224	10389	1.81%	0.215%
20	11.622	3281	3291	3307	rVV	248394	384422	66.83%	7.974%




Sum of corrected areas: 4820886

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021722\
Data File : VV024740.D
Acq On : 17 Feb 2022 22:20
Operator : SY/MD
Sample : N1522-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4M72

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

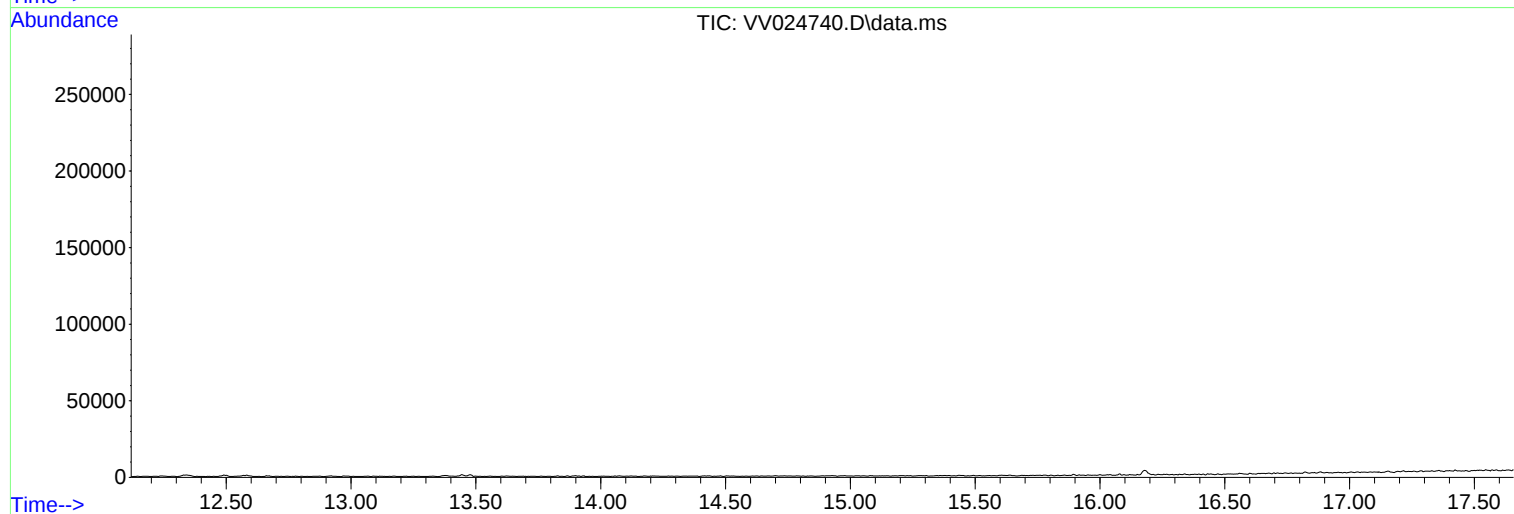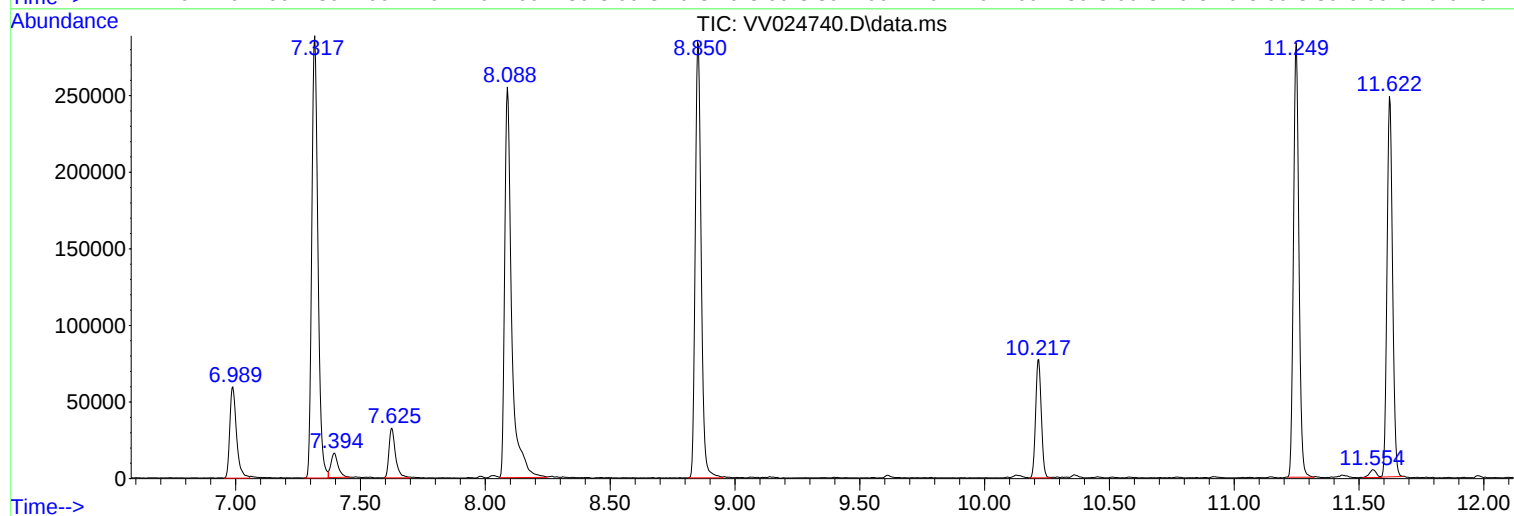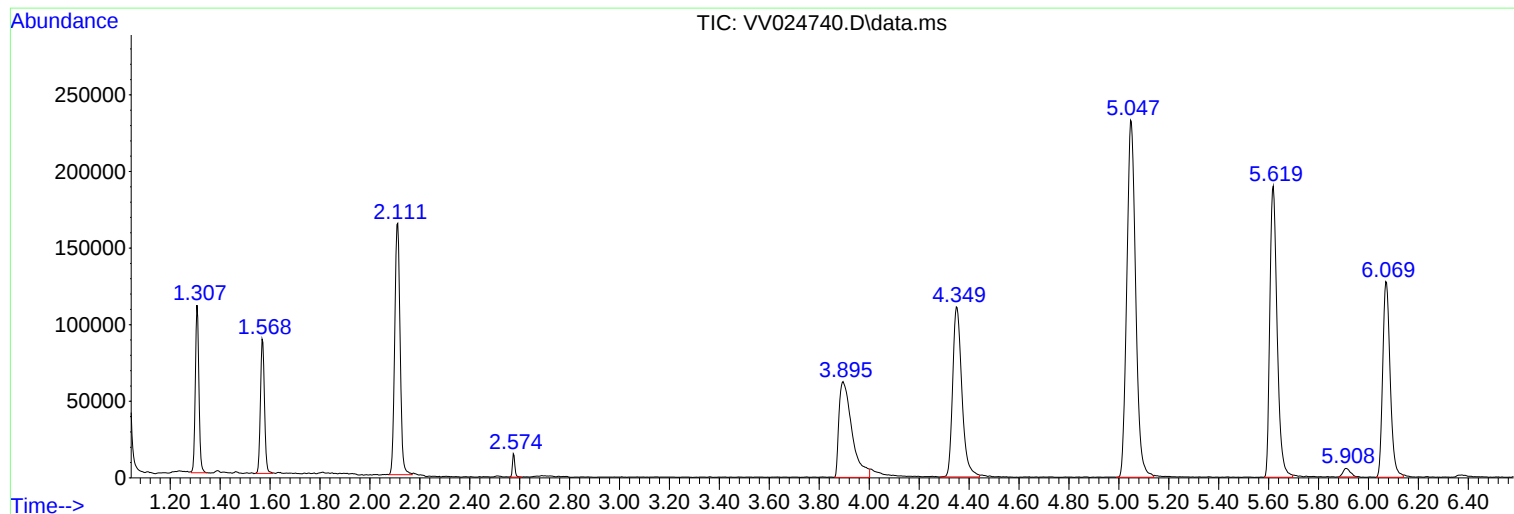

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021722\
Data File : VV024740.D
Acq On : 17 Feb 2022 22:20
Operator : SY/MD
Sample : N1522-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4M72

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021722\
Data File : VV024740.D
Acq On : 17 Feb 2022 22:20
Operator : SY/MD
Sample : N1522-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4M72

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc