
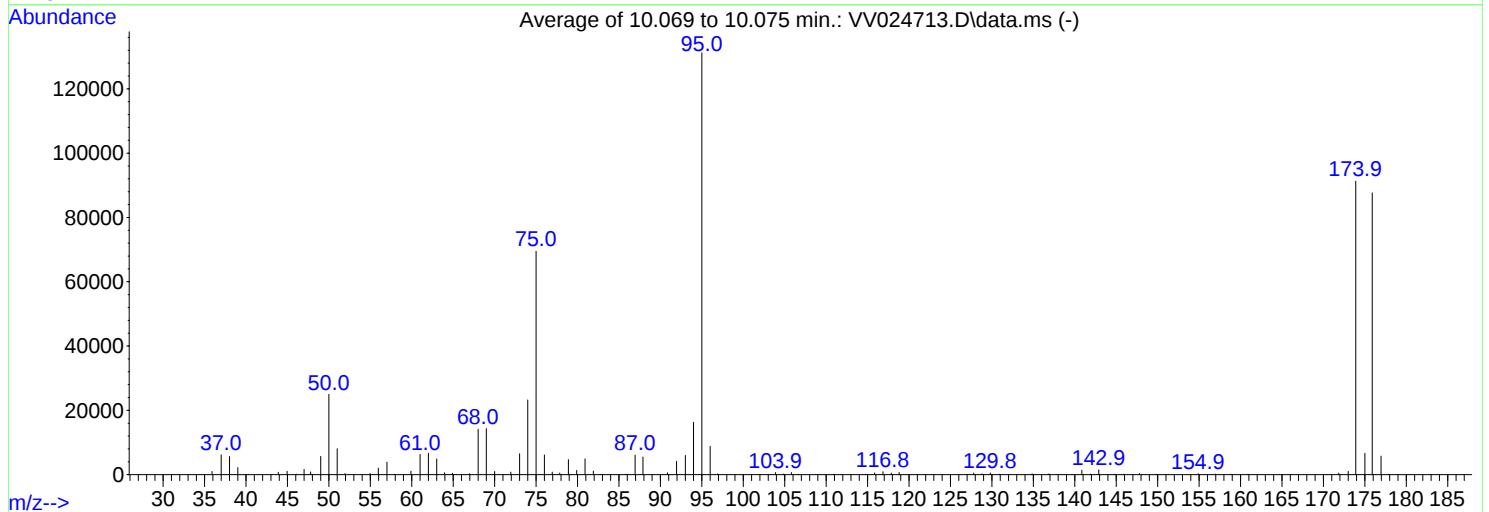


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021722\
Data File : VV024713.D
Acq On : 17 Feb 2022 09:01
Operator : SY/MD
Sample : BFB272
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB272

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Tue Feb 22 03:27:30 2022

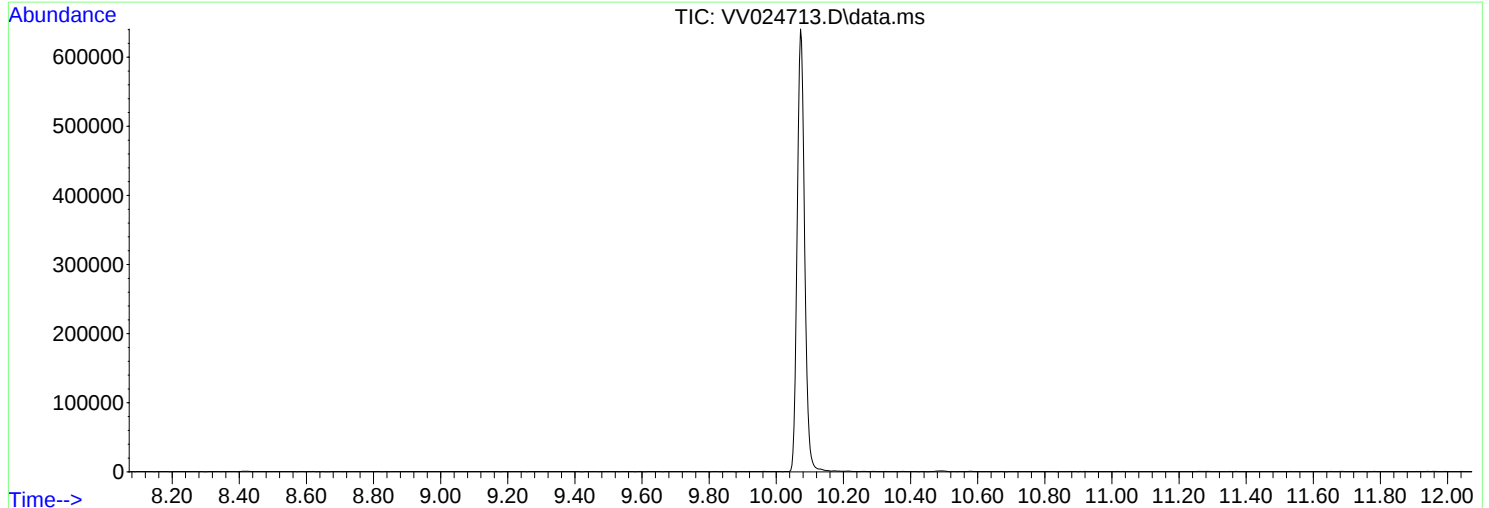

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	24976	PASS
75	95	30	80	52.9	69469	PASS
95	95	100	100	100.0	131205	PASS
96	95	5	9	6.7	8820	PASS
173	174	0.00	2	1.1	989	PASS
174	95	50	120	69.6	91261	PASS
175	174	5	9	7.3	6630	PASS
176	174	95	105	96.0	87640	PASS
177	176	5	10	6.6	5752	PASS

m/z	Abundance
39.90	117.0
44.00	342.0

Instrument :
MSVOA_V
ClientSampleId :
BFB272

m/z	Abundance
35.90	1013.0
37.00	6044.0
38.00	5642.0
39.00	2086.0
39.90	213.0
43.90	962.0
44.90	1063.0
46.00	142.0
47.00	1565.0
47.80	854.0
49.00	5633.0
50.00	24288.0
51.00	7904.0
51.90	395.0
55.00	340.0
56.00	2006.0
57.00	3687.0
57.90	160.0
59.90	1102.0
61.00	6255.0
62.00	6568.0
63.00	4785.0
64.00	612.0
64.90	496.0
67.00	345.0
68.00	13461.0
69.00	13267.0
70.00	1014.0
72.00	698.0
73.00	6157.0
74.00	22144.0
75.00	67696.0
76.00	5944.0
77.00	775.0
77.80	521.0
78.90	4559.0
79.90	1359.0
80.90	4856.0
81.90	1064.0
82.80	119.0
85.90	173.0
87.00	5737.0
87.90	5362.0
90.80	587.0
92.00	4085.0
93.00	5607.0
94.00	15648.0
95.00	125968.0
96.00	8865.0
96.90	292.0
103.90	561.0
104.80	209.0
105.80	605.0
110.80	120.0
111.80	111.0
113.00	128.0
114.70	156.0
115.90	484.0
116.80	793.0
117.80	457.0
118.80	671.0
127.80	486.0
128.80	218.0
129.80	493.0
130.90	134.0
134.90	222.0
136.90	223.0
140.80	1408.0
141.80	188.0
142.90	1447.0
144.80	121.0
145.90	199.0
147.80	318.0
149.00	116.0
149.80	179.0
154.90	288.0
156.90	188.0
158.80	150.0
160.90	127.0
171.80	508.0
173.00	874.0
173.90	85760.0
175.00	6417.0
175.90	81576.0
176.90	5468.0
177.90	160.0

Instrument :
MSVOA_V
ClientSampleId :
BFB272

m/z	Abundance
35.90	1039.0
37.00	6392.0
38.00	5837.0
39.00	2290.0
39.90	232.0
43.90	1118.0
45.00	1060.0
46.00	189.0
47.00	1728.0
47.80	951.0
49.00	6002.0
50.00	25816.0
51.00	8331.0
52.00	385.0
53.00	111.0
54.90	351.0
55.90	2112.0
57.00	4023.0
57.90	158.0
59.90	1089.0
61.00	6467.0
62.00	6868.0
63.00	5000.0
64.00	624.0
64.90	503.0
66.90	310.0
68.00	14803.0
69.00	14894.0
70.00	1060.0
72.00	840.0
73.00	6739.0
74.00	24080.0
75.00	71720.0
76.00	6374.0
77.00	817.0
77.80	473.0
78.90	4883.0
79.90	1413.0
80.90	5046.0
81.90	1109.0
83.00	126.0
85.90	165.0
86.90	6396.0
87.90	5697.0
90.80	616.0
91.90	4305.0
93.00	6193.0
94.00	16736.0
95.00	135616.0
96.00	9188.0
96.90	263.0
103.90	668.0
104.90	212.0
105.80	664.0
106.70	119.0
110.80	127.0
111.80	118.0
113.00	131.0
114.80	167.0
115.80	608.0
116.90	934.0
117.90	515.0
118.80	724.0
127.80	533.0
128.80	230.0
129.80	563.0
130.90	163.0
134.90	239.0
136.90	282.0
140.90	1479.0
141.90	203.0
142.90	1564.0
144.90	139.0
145.90	220.0
147.80	369.0
149.00	134.0
149.80	154.0
153.00	120.0
154.90	336.0
157.00	177.0
158.90	156.0
160.90	145.0
170.50	105.0
171.80	527.0
173.00	1026.0
173.90	94400.0
175.00	6863.0
175.90	91024.0
177.00	5933.0
177.90	183.0

Instrument :
MSVOA_V
ClientSampleId :
BFB272

m/z	Abundance
35.90	992.0
37.00	6052.0
38.00	5372.0
39.00	2201.0
39.90	233.0
43.90	1158.0
45.00	990.0
46.10	189.0
47.00	1597.0
47.80	829.0
49.00	5466.0
50.00	24824.0
51.00	7975.0
52.00	344.0
53.00	110.0
54.90	312.0
55.90	2009.0
57.00	3924.0
57.90	148.0
59.90	1027.0
61.00	6177.0
62.00	6510.0
63.00	4831.0
63.90	574.0
64.90	404.0
66.90	307.0
68.00	14198.0
69.00	14907.0
70.00	988.0
71.90	862.0
73.00	6468.0
74.00	23464.0
75.00	68992.0
76.00	6060.0
76.90	846.0
77.90	502.0
78.90	4636.0
79.90	1311.0
80.90	4843.0
81.90	1052.0
83.00	127.0
85.80	149.0
86.90	6151.0
87.90	5412.0
90.90	564.0
91.90	4057.0
93.00	6108.0
94.00	16520.0
95.00	132032.0
96.00	8406.0
96.90	199.0
103.90	701.0
104.90	187.0
105.80	649.0
106.60	155.0
110.90	124.0
111.80	117.0
112.90	117.0
114.80	155.0
115.80	617.0
116.90	951.0
117.90	569.0
118.80	739.0
127.80	523.0
128.80	261.0
129.80	544.0
130.90	180.0
134.80	245.0
136.90	315.0
139.80	104.0
140.90	1330.0
142.00	210.0
142.90	1529.0
144.90	159.0
146.00	215.0
147.80	361.0
149.00	125.0
149.80	115.0
152.90	132.0
154.90	335.0
157.00	167.0
158.90	154.0
160.90	139.0
171.90	542.0
173.00	1067.0
173.90	93624.0
175.00	6609.0
175.90	90320.0
177.00	5855.0
177.90	167.0

Instrument :
MSVOA_V
ClientSampleId :
BFB272