
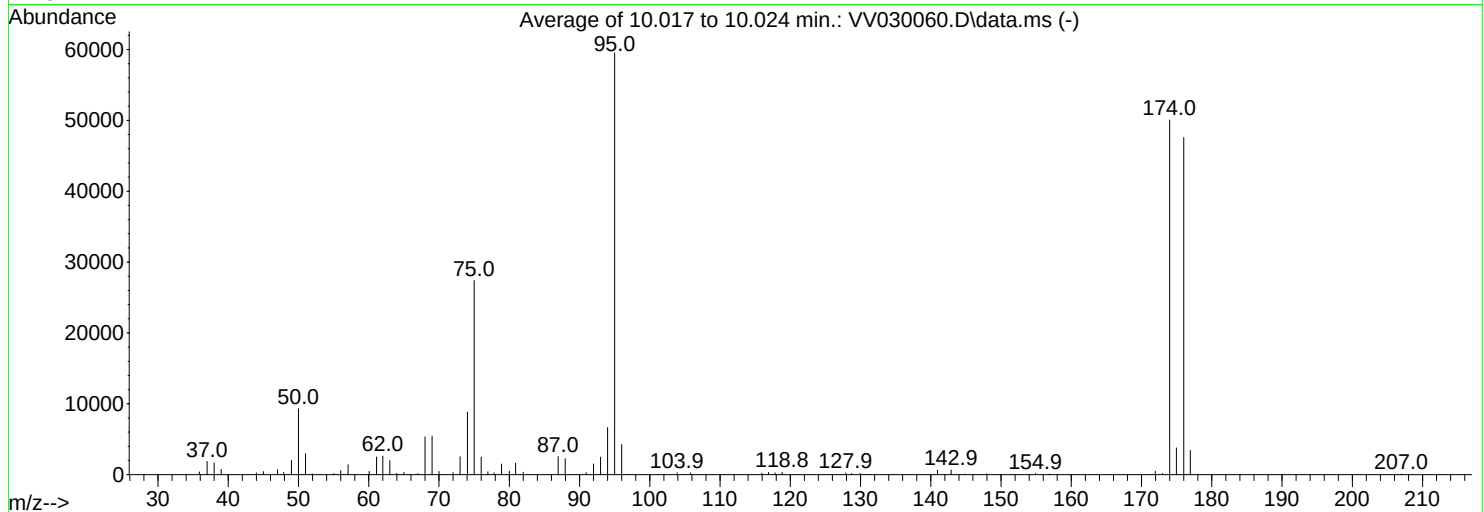


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021723\
Data File : VV030060.D
Acq On : 17 Feb 2023 09:41
Operator : SY/MD
Sample : BFB363
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB363

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM021723WMA.M
Title : VOC Analysis
Last Update : Mon Feb 20 22:59:49 2023

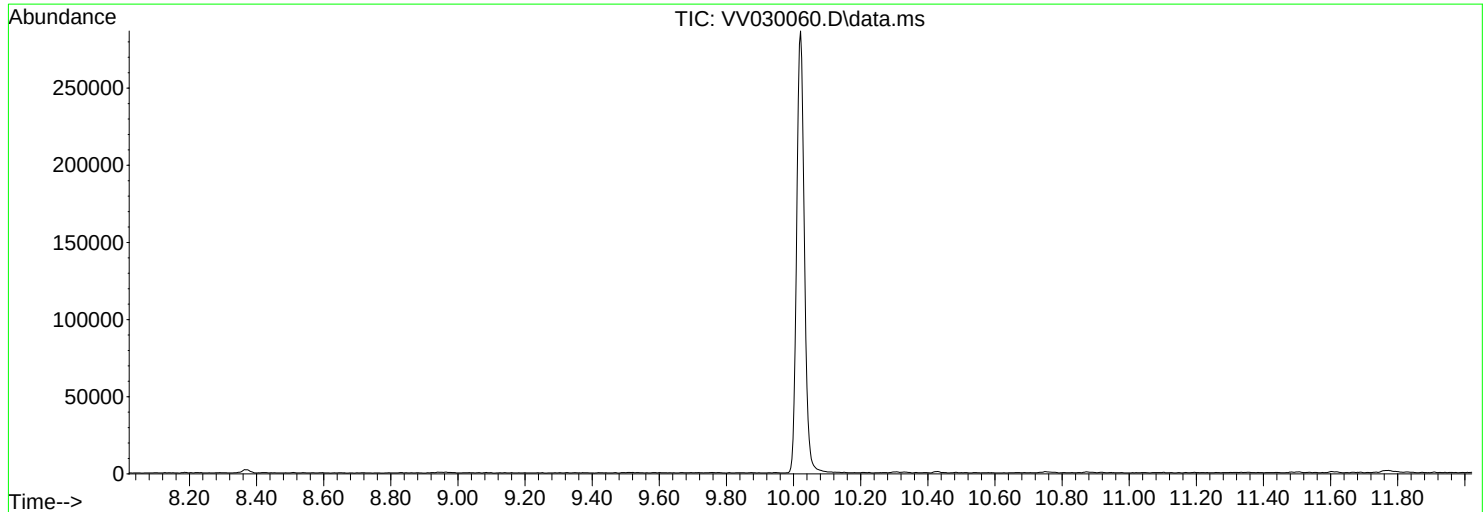

AutoFind: Scans 2792, 2793, 2794; Background Corrected with Scan 2780

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.6	9311	PASS
75	95	30	80	46.0	27400	PASS
95	95	100	100	100.0	59531	PASS
96	95	5	9	7.1	4252	PASS
173	174	0.00	2	0.3	151	PASS
174	95	50	120	84.1	50053	PASS
175	174	5	9	7.5	3762	PASS
176	174	95	105	95.1	47589	PASS
177	176	5	10	7.2	3431	PASS

m/z	Abundance
40.00	180.0
44.00	511.0

Instrument :
MSVOA_V
ClientSampleId :
BFB363

m/z	Abundance
35.90	393.0
37.00	1864.0
38.00	1758.0
39.00	762.0
39.90	189.0
44.00	745.0
45.00	507.0
47.00	684.0
47.90	315.0
49.00	1957.0
50.00	9512.0
51.00	3029.0
52.00	145.0
55.00	168.0
56.00	556.0
57.10	1516.0
60.10	454.0
61.10	2531.0
62.00	2633.0
63.00	1998.0
64.00	205.0
65.00	276.0
66.90	133.0
68.00	5297.0
69.00	5457.0
70.00	462.0
72.00	305.0
73.00	2363.0
74.00	9131.0
75.00	27768.0
76.00	2560.0
76.90	434.0
77.80	225.0
78.90	1473.0
80.00	513.0
80.90	1648.0
82.00	314.0
85.90	126.0
86.90	2668.0
88.00	2176.0
90.90	296.0
92.00	1494.0
93.00	2460.0
94.00	6913.0
95.00	60000.0
96.00	4288.0
97.00	131.0
103.90	258.0
104.90	114.0
105.80	201.0
115.90	226.0
116.90	343.0
117.80	280.0
118.80	358.0
127.90	266.0
128.70	115.0
130.00	160.0
141.00	561.0
142.90	628.0
144.80	143.0
147.90	144.0
154.90	124.0
156.90	152.0
171.90	455.0
173.00	452.0
174.00	49256.0
174.90	3633.0
176.00	46472.0
177.00	3396.0

Instrument :
MSVOA_V
ClientSampleId :
BFB363

m/z	Abundance
35.90	379.0
37.00	1908.0
38.00	1709.0
39.00	765.0
39.90	200.0
44.00	763.0
45.00	452.0
47.00	737.0
47.90	345.0
49.00	2106.0
50.00	9619.0
51.00	3066.0
52.00	132.0
55.00	150.0
56.00	583.0
57.10	1464.0
60.00	485.0
61.10	2558.0
62.00	2684.0
63.00	2070.0
64.00	202.0
65.00	327.0
67.00	133.0
68.00	5482.0
69.00	5615.0
70.00	467.0
72.00	295.0
73.00	2655.0
74.10	9016.0
75.00	28336.0
76.00	2548.0
76.90	430.0
77.80	247.0
78.90	1563.0
80.00	509.0
80.90	1661.0
82.00	361.0
87.00	2610.0
88.00	2327.0
90.90	316.0
92.00	1543.0
93.00	2542.0
94.00	6850.0
95.00	61472.0
96.00	4439.0
103.90	287.0
105.80	225.0
115.90	217.0
116.90	321.0
117.80	253.0
118.90	354.0
127.90	242.0
128.70	142.0
129.90	200.0
134.80	102.0
140.90	628.0
142.90	700.0
144.90	107.0
147.90	146.0
154.90	162.0
156.90	141.0
172.00	501.0
174.00	51680.0
174.90	3889.0
176.00	48904.0
176.90	3597.0
207.00	121.0

Instrument :
MSVOA_V
ClientSampleId :
BFB363

m/z	Abundance
35.90	363.0
37.00	1847.0
38.00	1573.0
39.00	697.0
39.90	204.0
44.00	782.0
45.00	342.0
47.00	698.0
47.90	320.0
49.00	1998.0
50.00	8802.0
51.00	2762.0
51.90	131.0
55.00	123.0
56.00	531.0
57.00	1242.0
60.00	480.0
61.10	2384.0
62.00	2536.0
63.00	1872.0
64.00	218.0
65.00	347.0
67.10	127.0
68.00	5182.0
69.00	5231.0
70.00	429.0
72.00	259.0
73.00	2600.0
74.10	8316.0
75.00	26096.0
76.00	2316.0
77.00	375.0
77.90	247.0
78.90	1437.0
80.00	462.0
80.90	1561.0
82.00	372.0
87.00	2380.0
87.90	2280.0
91.00	283.0
92.00	1531.0
93.00	2366.0
94.00	6140.0
95.00	57120.0
96.00	4030.0
103.90	267.0
105.80	241.0
116.00	189.0
116.90	303.0
117.90	205.0
118.90	307.0
127.90	203.0
128.70	124.0
129.90	199.0
130.90	116.0
134.80	106.0
140.90	643.0
142.90	633.0
147.90	129.0
154.90	159.0
172.00	502.0
174.00	49224.0
175.00	3763.0
176.00	47392.0
176.90	3301.0
207.00	119.0

Instrument :
MSVOA_V
ClientSampleId :
BFB363