

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW021822\
 Data File : VW024753.D
 Acq On : 18 Feb 2022 15:06
 Operator : SY/MD
 Sample : VIBLK257
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK256

Quant Time: Feb 19 00:45:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Feb 19 00:43:23 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	142465	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	139081	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	69253	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	52794	4.369	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	87.400%	
7) Chloroethane-d5	1.567	69	45503	4.590	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	91.800%	
11) 1,1-Dichloroethene-d2	2.111	63	72954	3.295	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	65.800%	
20) 2-Butanone-d5	3.886	46	107441	62.248	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	124.500%	
24) Chloroform-d	4.352	84	100937	5.353	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	107.000%	
26) 1,2-Dichloroethane-d4	5.034	65	45909	5.462	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	109.200%	
32) Benzene-d6	5.050	84	212365	5.293	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	105.800%	
36) 1,2-Dichloropropane-d6	6.069	67	64483	5.461	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	109.200%	
41) Toluene-d8	7.316	98	180655	4.955	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	99.200%	
43) trans-1,3-Dichloroprop...	7.625	79	19694	5.007	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	100.200%	
46) 2-Hexanone-d5	8.088	63	86741	56.042	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	112.080%	
56) 1,1,2,2-Tetrachloroeth...	10.213	84	38038	5.345	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	107.000%	
66) 1,2-Dichlorobenzene-d4	11.622	152	58685	4.897	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	98.000%	
Target Compounds						
					Qvalue	
25) Chloroform	4.384	83	3701	0.179	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021822\
Data File : VV024753.D
Acq On : 18 Feb 2022 15:06
Operator : SY/MD
Sample : VIBLK257
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK256

Quant Time: Feb 19 00:45:18 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Feb 19 00:43:23 2022
Response via : Initial Calibration

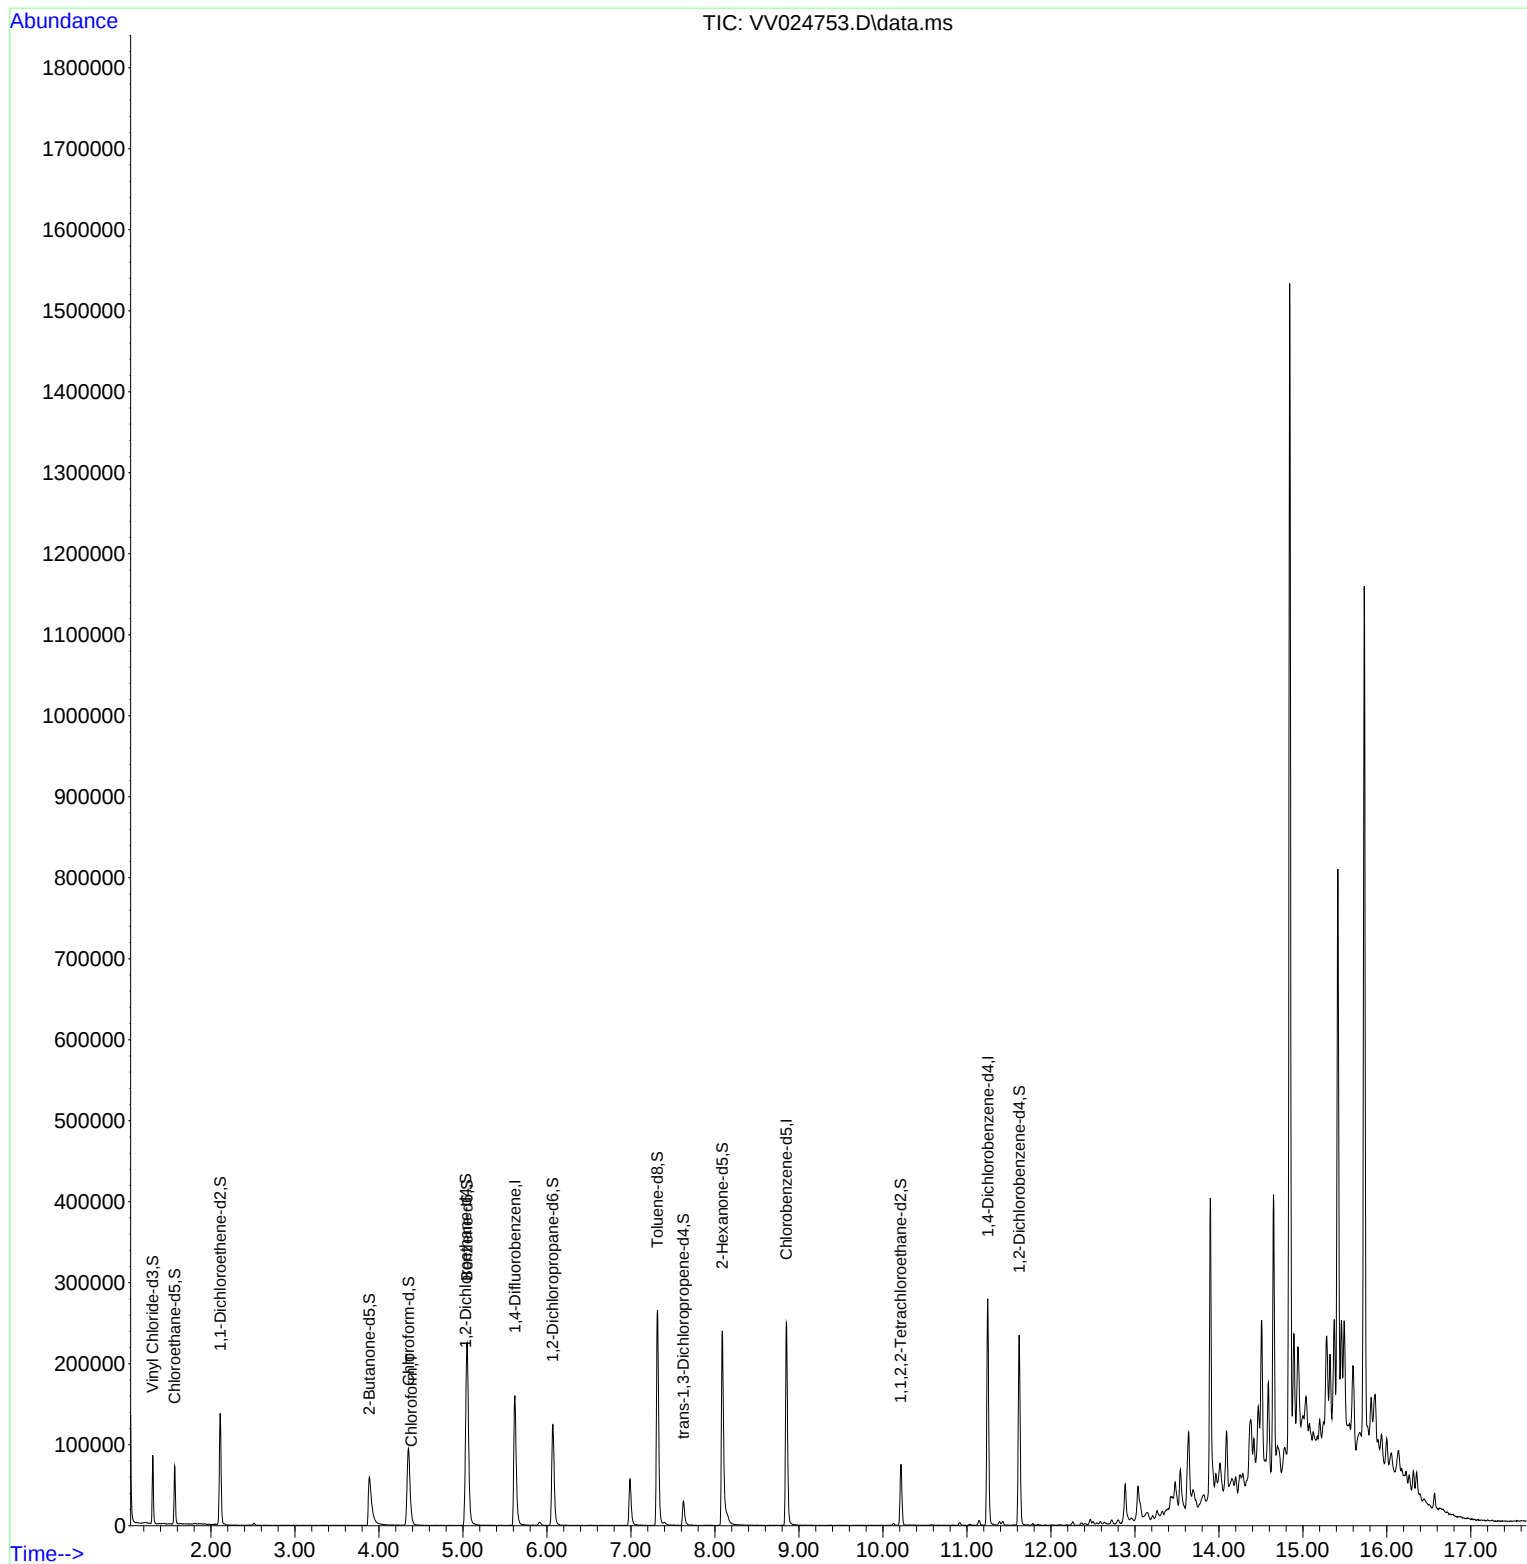

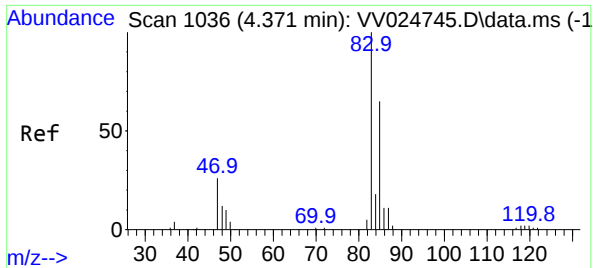

#25
Chloroform
Concen: 0.179 ug/L
RT: 4.384 min Scan# 10
Delta R.T. 0.013 min
Lab File: VV024753.D
Acq: 18 Feb 2022 15:06

Instrument :
MSVOA_V
ClientSampleId :
VIBLK256

Tgt Ion: 83 Resp: 3701
Ion Ratio Lower Upper
83 100
85 69.6 45.5 84.5

