

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW021822\
 Data File : VW024756.D
 Acq On : 18 Feb 2022 16:16
 Operator : SY/MD
 Sample : VIBLK258
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK257

Quant Time: Feb 19 00:45:55 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Feb 19 00:43:23 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	185205	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	170498	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	76527	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	62139	3.956	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	79.200%
7) Chloroethane-d5	1.568	69	54347	4.217	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	84.400%
11) 1,1-Dichloroethene-d2	2.111	63	86022	2.988	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	59.800%#
20) 2-Butanone-d5	3.886	46	108858	48.514	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	97.020%
24) Chloroform-d	4.352	84	107812	4.398	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.000%
26) 1,2-Dichloroethane-d4	5.034	65	50908	4.659	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.200%
32) Benzene-d6	5.050	84	225946	4.594	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.800%
36) 1,2-Dichloropropane-d6	6.069	67	69308	4.788	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	95.800%
41) Toluene-d8	7.317	98	197292	4.414	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.200%
43) trans-1,3-Dichloroprop...	7.625	79	20652	4.283	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.600%
46) 2-Hexanone-d5	8.088	63	86898	45.798	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	91.600%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	39164	4.489	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	89.800%
66) 1,2-Dichlorobenzene-d4	11.622	152	61743	4.663	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	93.200%
Target Compounds					Qvalue	
25) Chloroform	4.381	83	3861	0.143	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021822\
Data File : VV024756.D
Acq On : 18 Feb 2022 16:16
Operator : SY/MD
Sample : VIBLK258
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK257

Quant Time: Feb 19 00:45:55 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Feb 19 00:43:23 2022
Response via : Initial Calibration

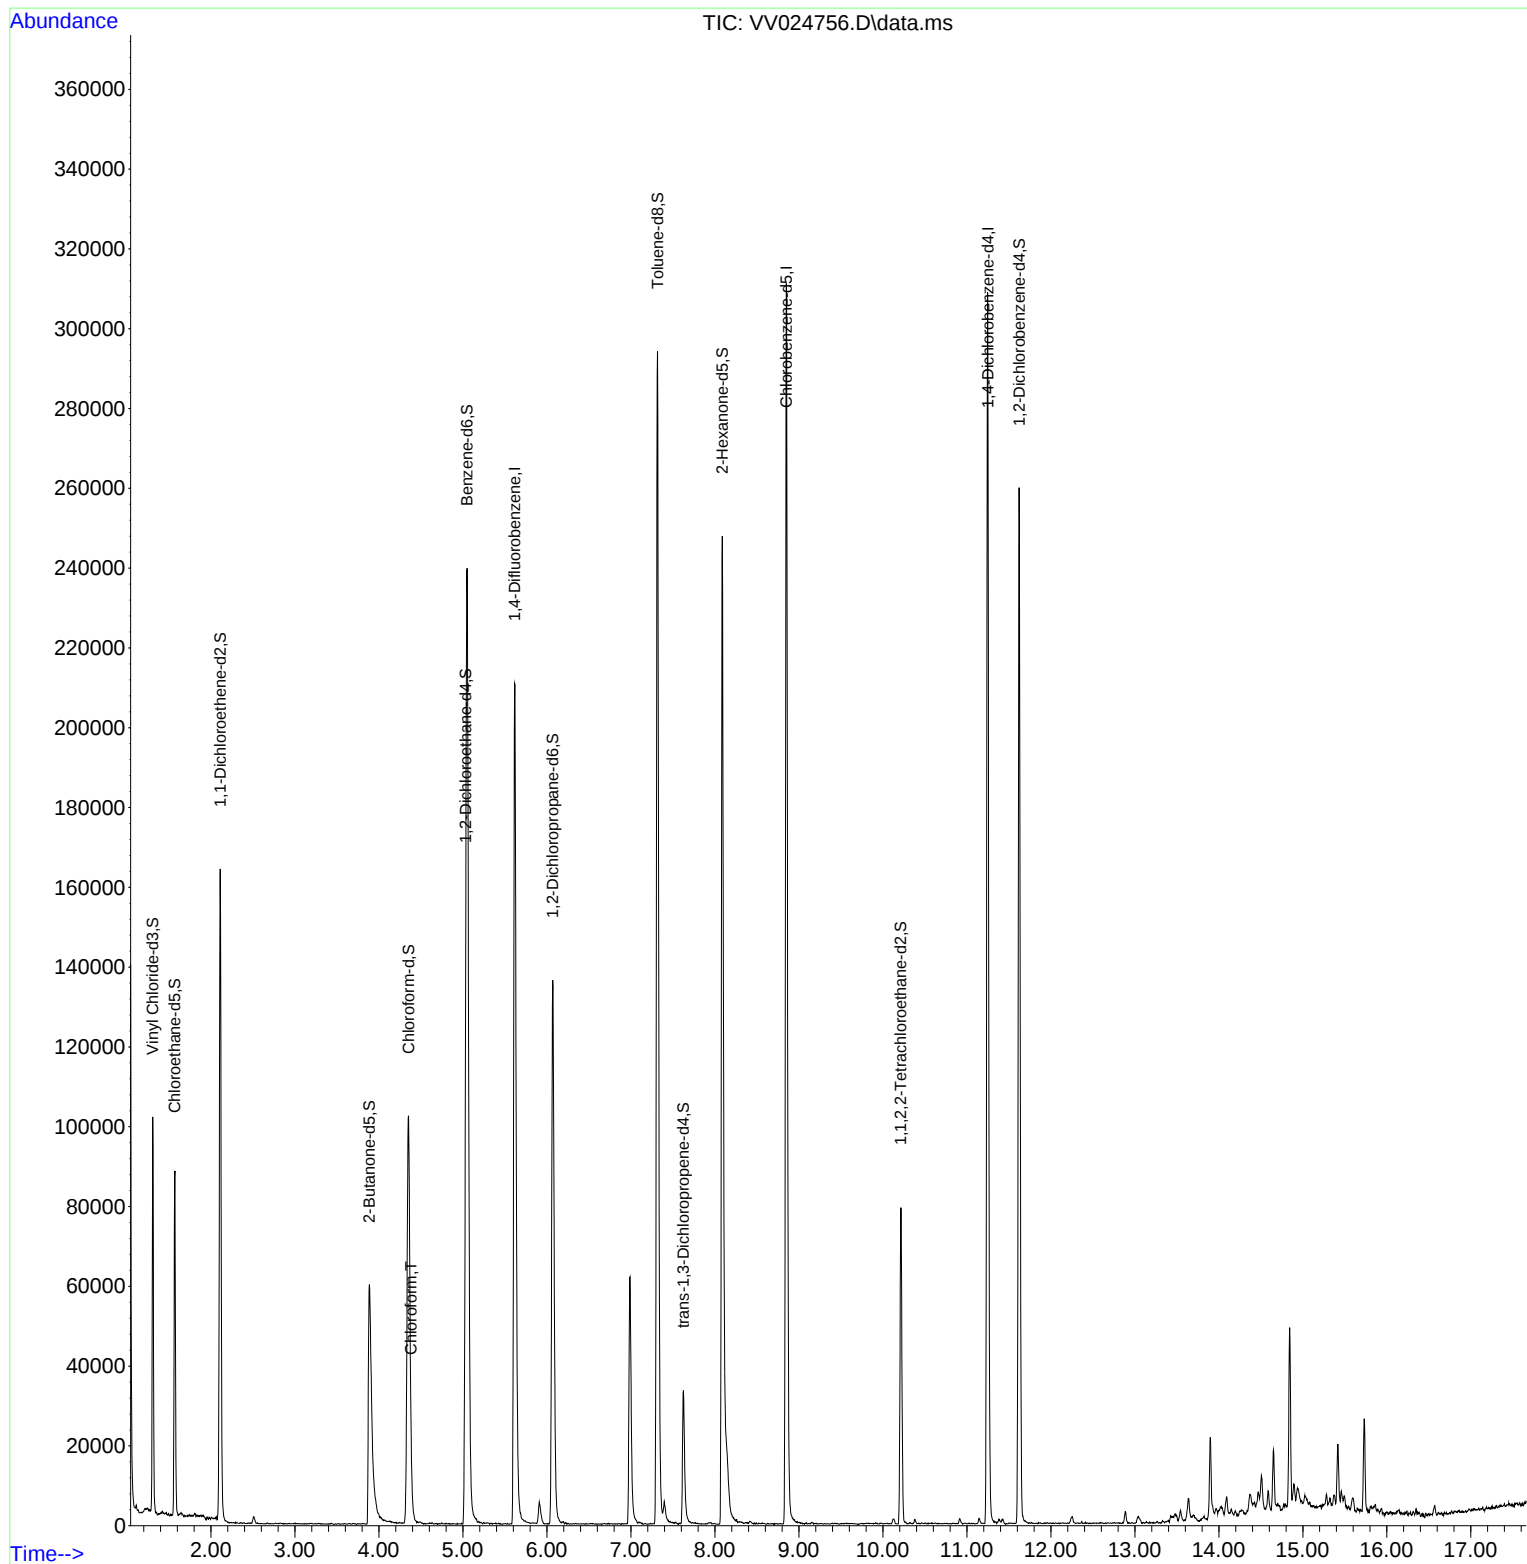

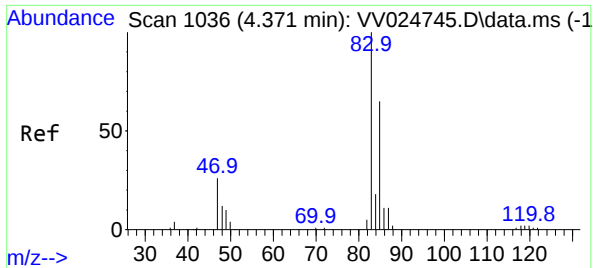

#25
Chloroform
Concen: 0.143 ug/L
RT: 4.381 min Scan# 10
Delta R.T. 0.010 min
Lab File: VV024756.D
Acq: 18 Feb 2022 16:16

Instrument :
MSVOA_V
ClientSampleId :
VIBLK257

Tgt Ion: 83 Resp: 3861
Ion Ratio Lower Upper
83 100
85 70.6 45.5 84.5

