

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW021822\
 Data File : VW024760.D
 Acq On : 18 Feb 2022 17:50
 Operator : SY/MD
 Sample : VIBLK259
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK258

Quant Time: Feb 19 00:46:51 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Feb 19 00:43:23 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	176877	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	162098	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	74423	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	57580	3.838	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	76.800%
7) Chloroethane-d5	1.571	69	50659	4.116	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	82.400%
11) 1,1-Dichloroethene-d2	2.111	63	78596	2.859	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	57.200%#
20) 2-Butanone-d5	3.889	46	111606	52.081	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	104.160%
24) Chloroform-d	4.352	84	96586	4.126	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	82.600%
26) 1,2-Dichloroethane-d4	5.034	65	47955	4.596	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.000%
32) Benzene-d6	5.050	84	207916	4.446	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.000%
36) 1,2-Dichloropropane-d6	6.069	67	64141	4.661	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	93.200%
41) Toluene-d8	7.317	98	182139	4.286	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.800%
43) trans-1,3-Dichloroprop...	7.625	79	20752	4.527	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.600%
46) 2-Hexanone-d5	8.088	63	88156	48.869	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	97.740%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	38277	4.615	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.400%
66) 1,2-Dichlorobenzene-d4	11.622	152	59857	4.648	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	93.000%
Target Compounds					Qvalue	
25) Chloroform	4.378	83	6969	0.271	ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021822\
Data File : VV024760.D
Acq On : 18 Feb 2022 17:50
Operator : SY/MD
Sample : VIBLK259
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK258

Quant Time: Feb 19 00:46:51 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Feb 19 00:43:23 2022
Response via : Initial Calibration

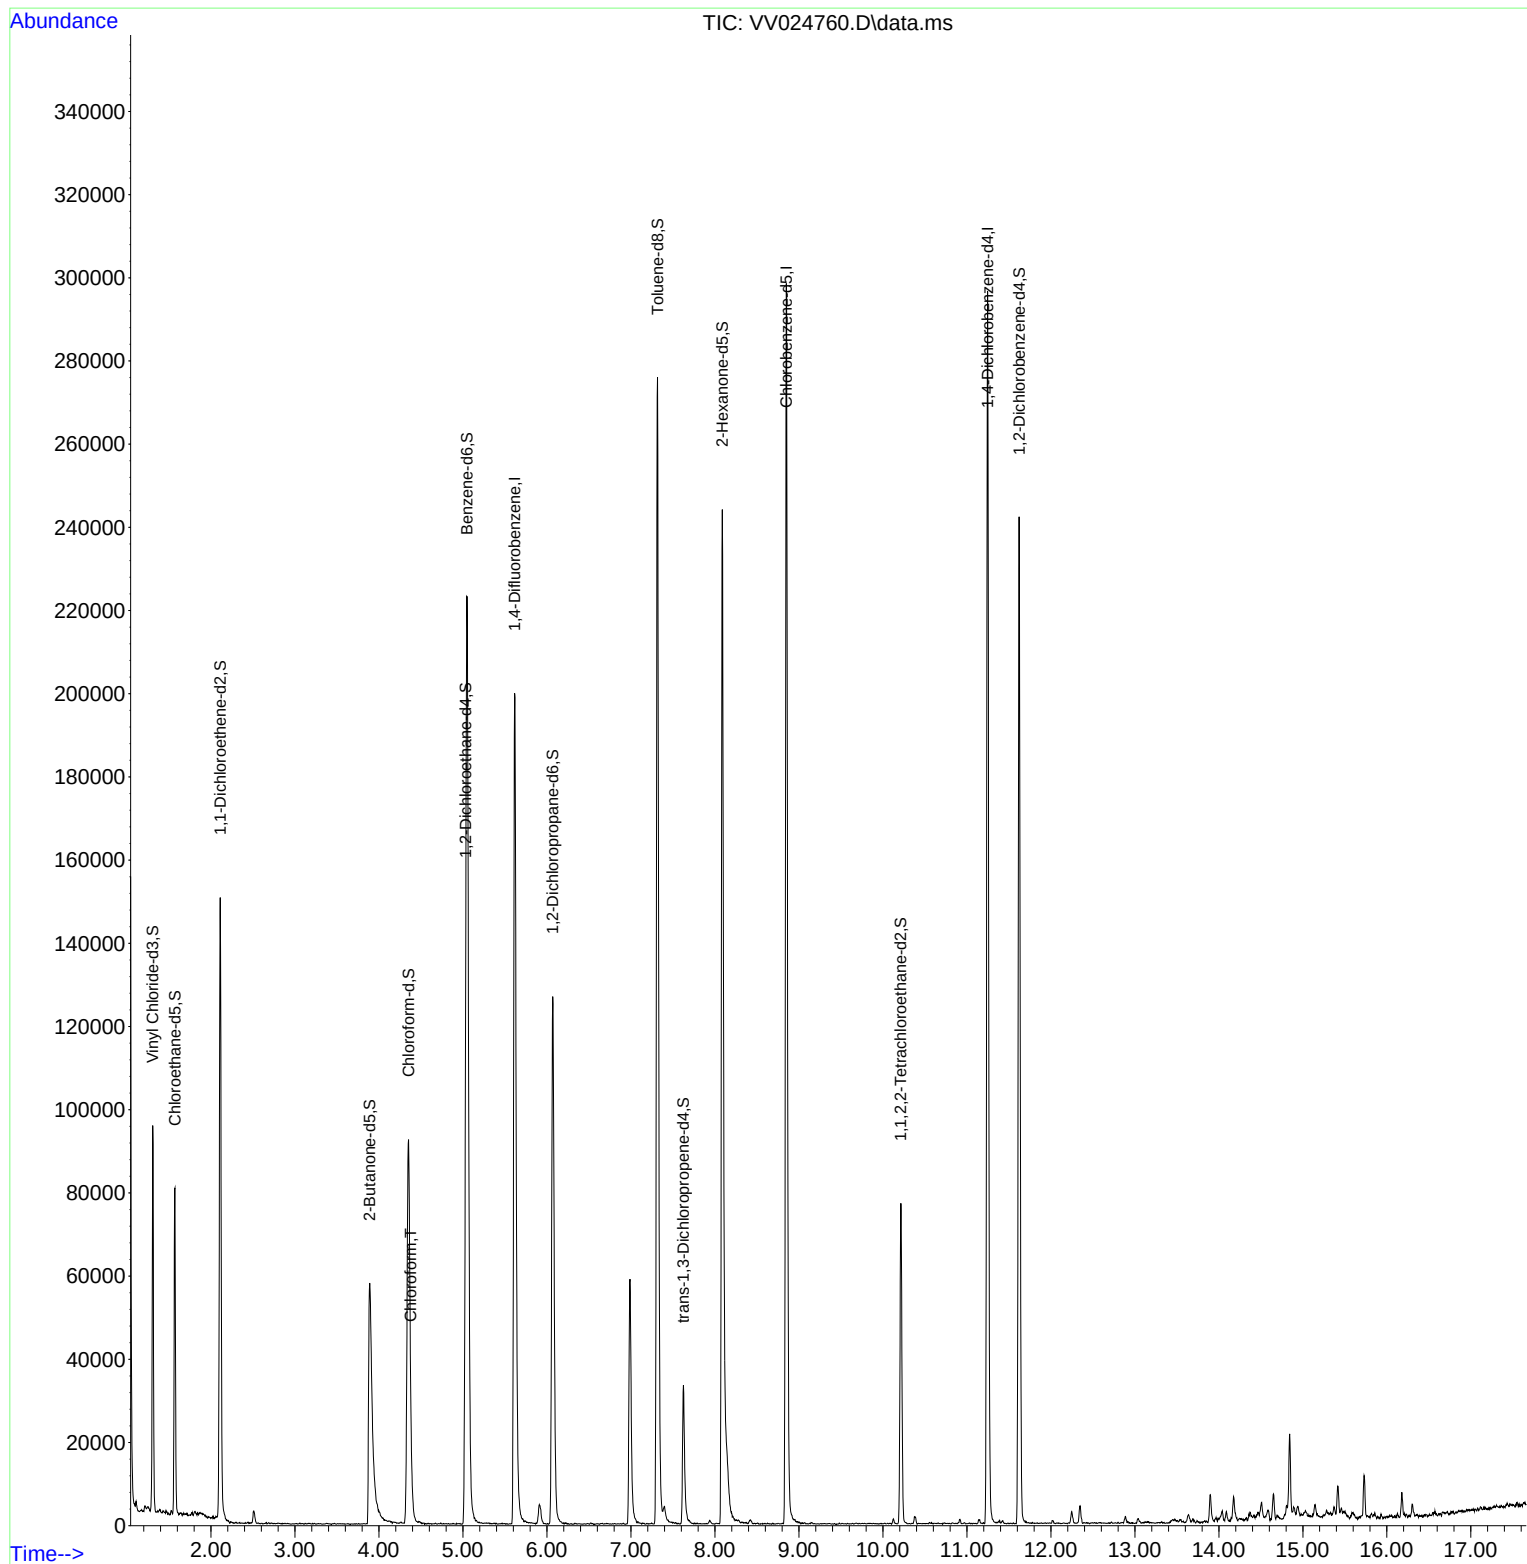

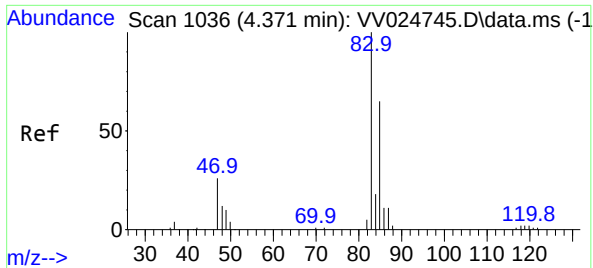

#25
 Chloroform
 Concen: 0.271 ug/L
 RT: 4.378 min Scan# 10
 Delta R.T. 0.007 min
 Lab File: VV024760.D
 Acq: 18 Feb 2022 17:50

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK258

Tgt Ion: 83 Resp: 6969
 Ion Ratio Lower Upper
 83 100
 85 71.1 45.5 84.5

