

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW021822\
 Data File : VW024764.D
 Acq On : 18 Feb 2022 19:24
 Operator : SY/MD
 Sample : N1510-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4M30

Quant Time: Feb 19 15:40:49 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Feb 19 00:43:23 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	167738	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	153844	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	68535	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	58011	4.077	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	81.600%
7) Chloroethane-d5	1.571	69	52328	4.483	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	89.600%
11) 1,1-Dichloroethene-d2	2.111	63	79771	3.060	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	61.200%
20) 2-Butanone-d5	3.889	46	106500	52.406	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	104.820%
24) Chloroform-d	4.352	84	97077	4.373	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.400%
26) 1,2-Dichloroethane-d4	5.034	65	48093	4.860	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.200%
32) Benzene-d6	5.050	84	212619	4.791	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.800%
36) 1,2-Dichloropropane-d6	6.069	67	64635	4.949	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.000%
41) Toluene-d8	7.317	98	181298	4.496	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.000%
43) trans-1,3-Dichloroprop...	7.625	79	19871	4.567	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	91.400%
46) 2-Hexanone-d5	8.088	63	86562	50.559	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	101.120%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	38147	4.846	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	97.000%
66) 1,2-Dichlorobenzene-d4	11.622	152	59037	4.978	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.600%
Target Compounds					Qvalue	
25) Chloroform	4.381	83	6947	0.285	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021822\
Data File : VV024764.D
Acq On : 18 Feb 2022 19:24
Operator : SY/MD
Sample : N1510-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4M30

Quant Time: Feb 19 15:40:49 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Feb 19 00:43:23 2022
Response via : Initial Calibration

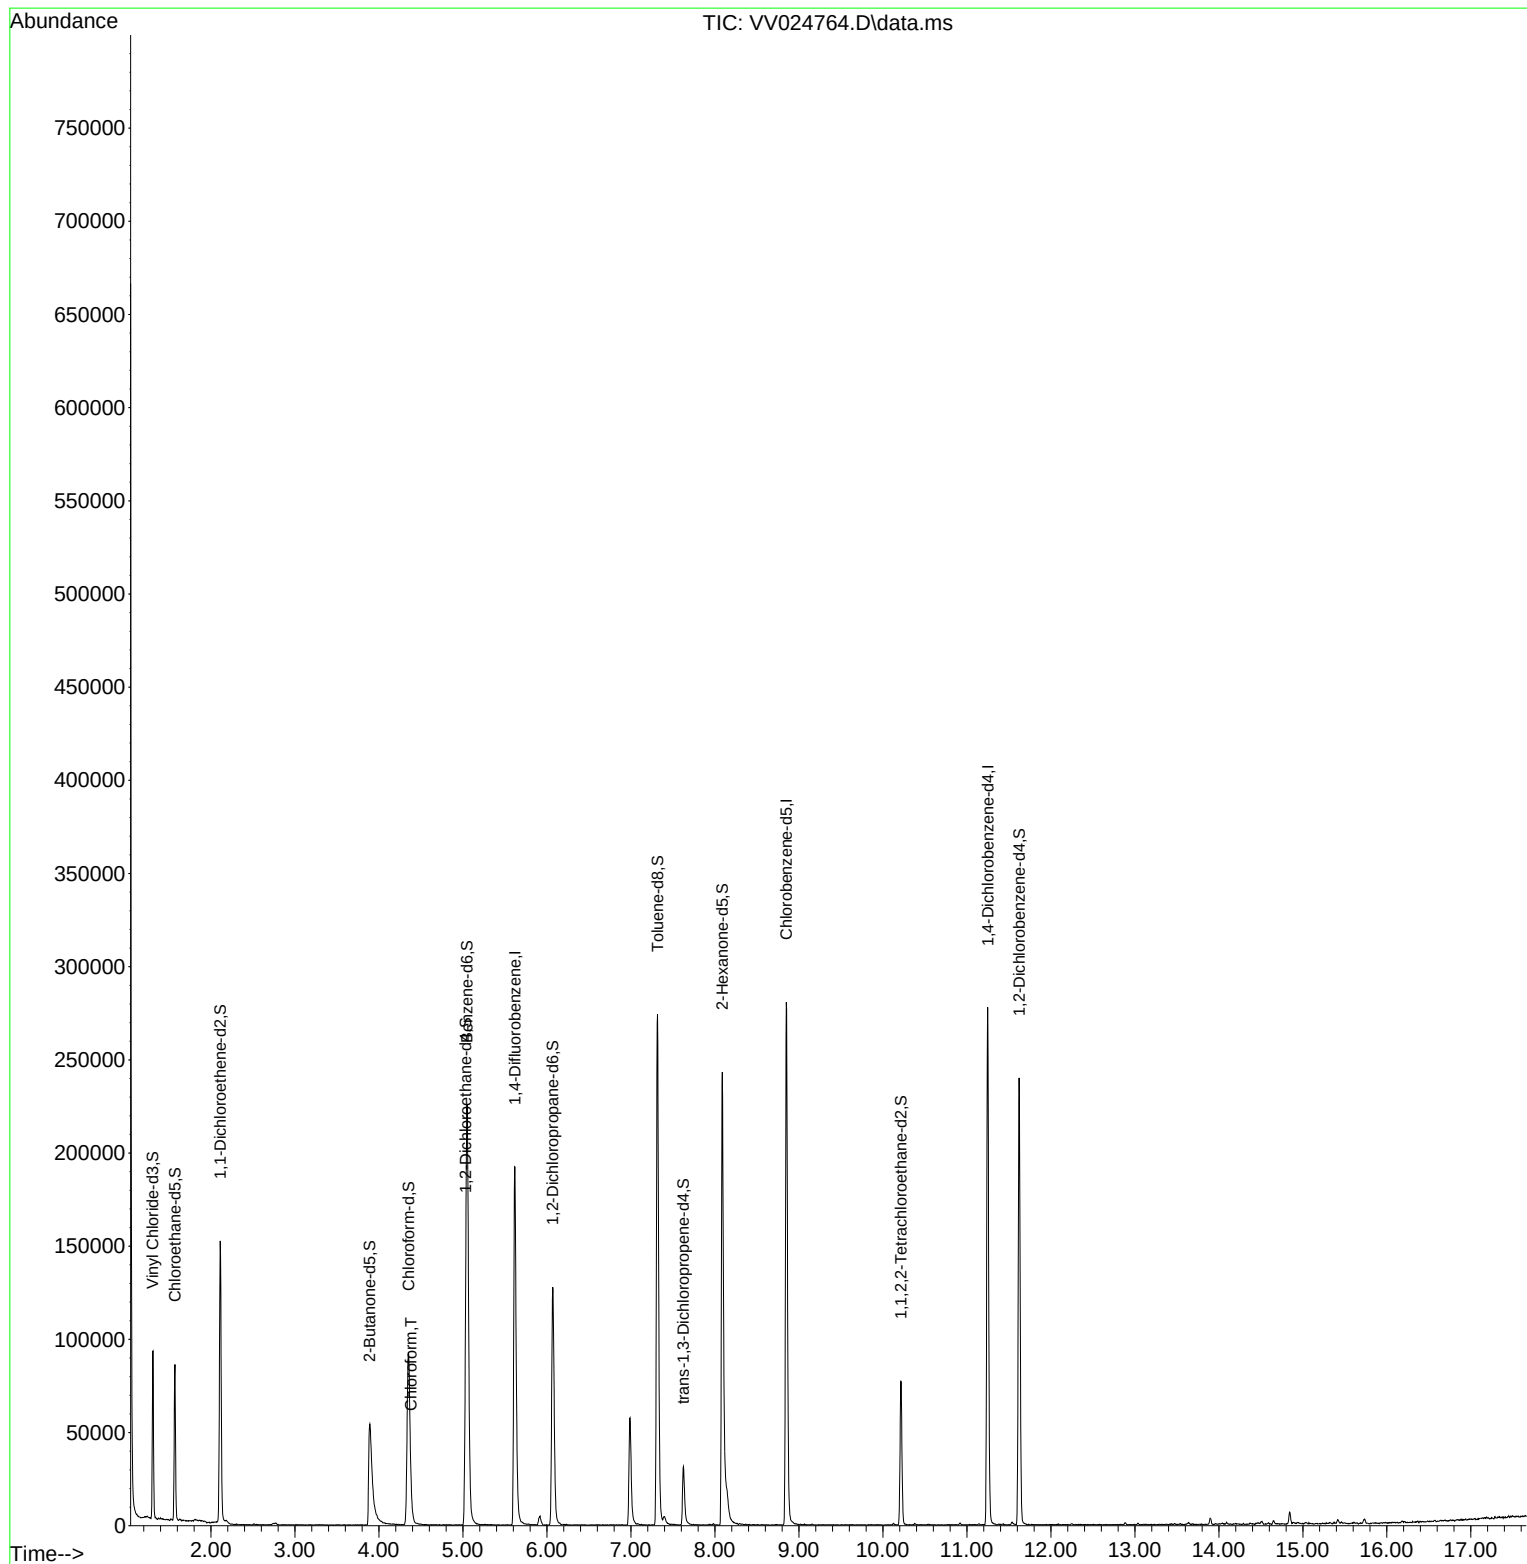

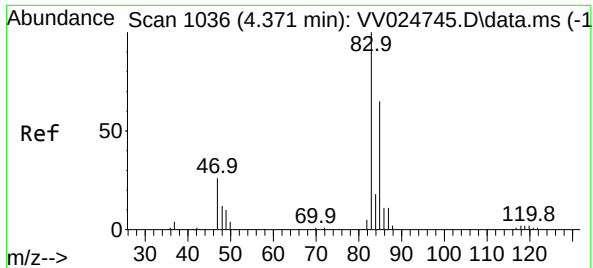

#25
Chloroform
Concen: 0.285 ug/L
RT: 4.381 min Scan# 10
Delta R.T. 0.006 min
Lab File: VV024764.D
Acq: 18 Feb 2022 19:24

Instrument :
MSVOA_V
ClientSampleId :
F4M30

Tgt Ion: 83 Resp: 6947
Ion Ratio Lower Upper
83 100
85 67.2 45.5 84.5

