

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021822\
 Data File : VV024765.D
 Acq On : 18 Feb 2022 19:47
 Operator : SY/MD
 Sample : N1510-13
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Feb 19 15:40:17 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Feb 19 00:43:23 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	139251	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	137597	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	66842	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	53746	4.550	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	91.000%	
7) Chloroethane-d5	1.571	69	49072	5.064	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	101.200%	
11) 1,1-Dichloroethene-d2	2.111	63	75364	3.482	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	69.600%	
20) 2-Butanone-d5	3.889	46	104518	61.952	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	123.900%	
24) Chloroform-d	4.352	84	96583	5.241	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	104.800%	
26) 1,2-Dichloroethane-d4	5.034	65	46603	5.673	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	113.400%	
32) Benzene-d6	5.053	84	201348	5.072	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	101.400%	
36) 1,2-Dichloropropane-d6	6.069	67	62063	5.313	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	106.200%	
41) Toluene-d8	7.317	98	174581	4.840	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	96.800%	
43) trans-1,3-Dichloroprop...	7.625	79	18561	4.770	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	95.400%	
46) 2-Hexanone-d5	8.088	63	80138	52.334	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	104.660%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	36330	5.160	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	103.200%	
66) 1,2-Dichlorobenzene-d4	11.622	152	56453	4.881	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	97.600%	
Target Compounds					Qvalue	
25) Chloroform	4.378	83	4286	0.212	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021822\
Data File : VV024765.D
Acq On : 18 Feb 2022 19:47
Operator : SY/MD
Sample : N1510-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Time: Feb 19 15:40:17 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Feb 19 00:43:23 2022
Response via : Initial Calibration

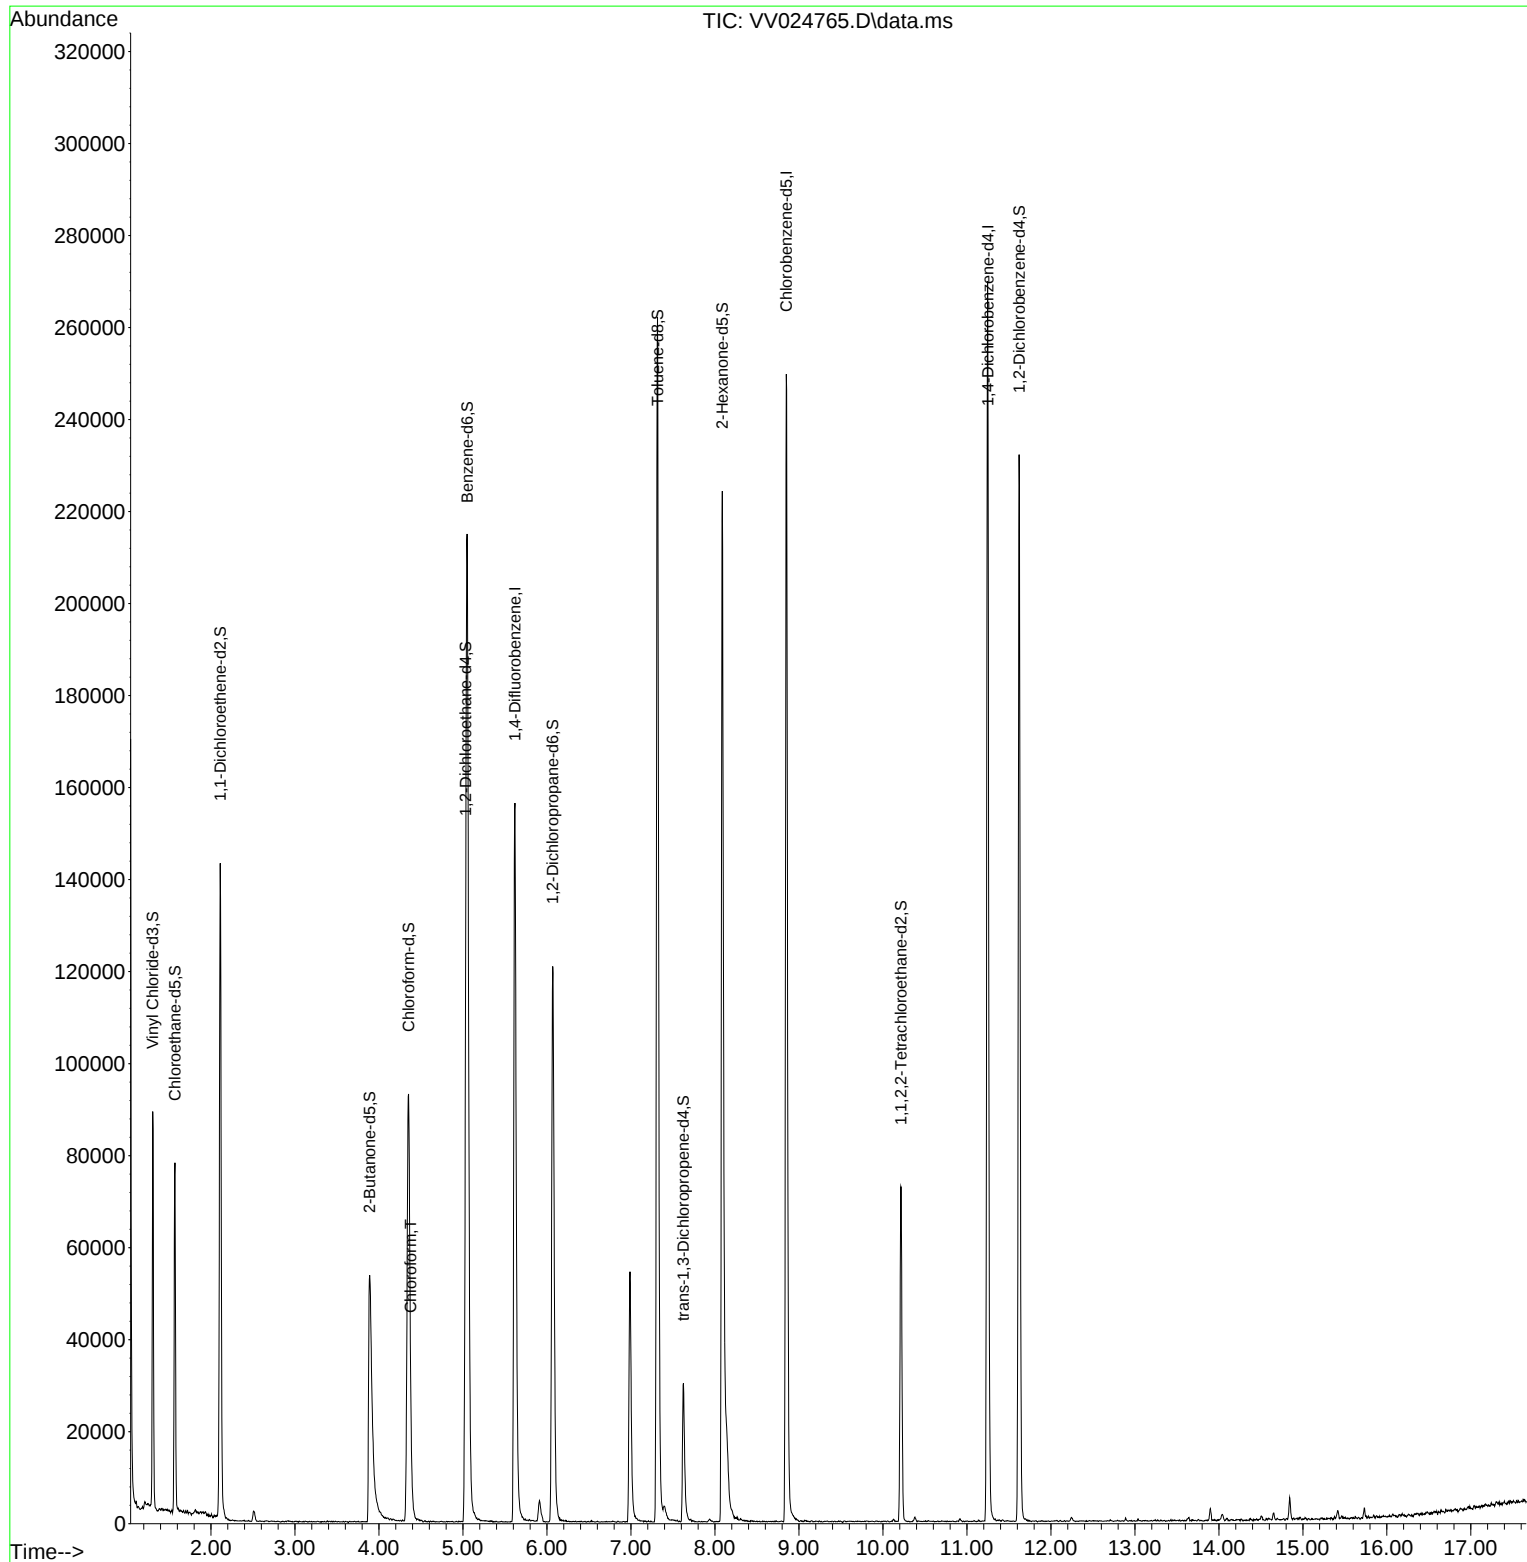

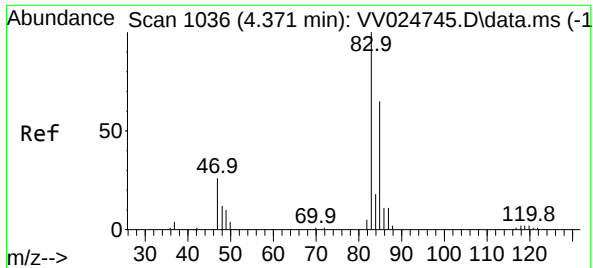

#25
 Chloroform
 Concen: 0.212 ug/L
 RT: 4.378 min Scan# 10
 Delta R.T. 0.003 min
 Lab File: VV024765.D
 Acq: 18 Feb 2022 19:47

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Tgt Ion: 83 Resp: 4286
 Ion Ratio Lower Upper
 83 100
 85 66.7 45.5 84.5

