

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021822\
 Data File : VV024746.D
 Acq On : 18 Feb 2022 12:09
 Operator : SY/MD
 Sample : VV0218WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK308

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV024746.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	94	rVB	108598	105659	18.45%	2.302%
2	1.571	156	165	176	rBV	86266	98262	17.16%	2.140%
3	2.108	320	332	359	rVB	169044	246830	43.11%	5.377%
4	2.510	449	457	467	rVB3	4201	7200	1.26%	0.157%
5	3.895	878	888	927	rBV	43079	157073	27.43%	3.422%
6	4.346	1011	1028	1056	rBV	97307	245760	42.92%	5.354%
7	5.043	1229	1245	1281	rBV2	231965	572567	100.00%	12.473%
8	5.612	1411	1422	1449	rBV	190787	387398	67.66%	8.439%
9	5.908	1504	1514	1527	rBV4	5390	10753	1.88%	0.234%
10	6.066	1550	1563	1593	rBV	128987	267393	46.70%	5.825%
11	6.985	1838	1849	1870	rBV	59483	111252	19.43%	2.423%
12	7.313	1938	1951	1970	rBV	284312	498150	87.00%	10.851%
13	7.394	1971	1976	1989	rVB3	3533	6560	1.15%	0.143%
14	7.622	2037	2047	2072	rBV	33299	59019	10.31%	1.286%
15	8.088	2179	2192	2229	rBV	214526	434610	75.91%	9.467%
16	8.850	2417	2429	2450	rBV	290230	465457	81.29%	10.139%
17	10.213	2841	2853	2872	rBV	73067	113320	19.79%	2.469%
18	11.246	3163	3174	3195	rBV	273371	425843	74.37%	9.276%
19	11.622	3280	3291	3313	rBV	243231	377504	65.93%	8.223%




Sum of corrected areas: 4590610

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021822\
Data File : VV024746.D
Acq On : 18 Feb 2022 12:09
Operator : SY/MD
Sample : VV0218WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK308

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

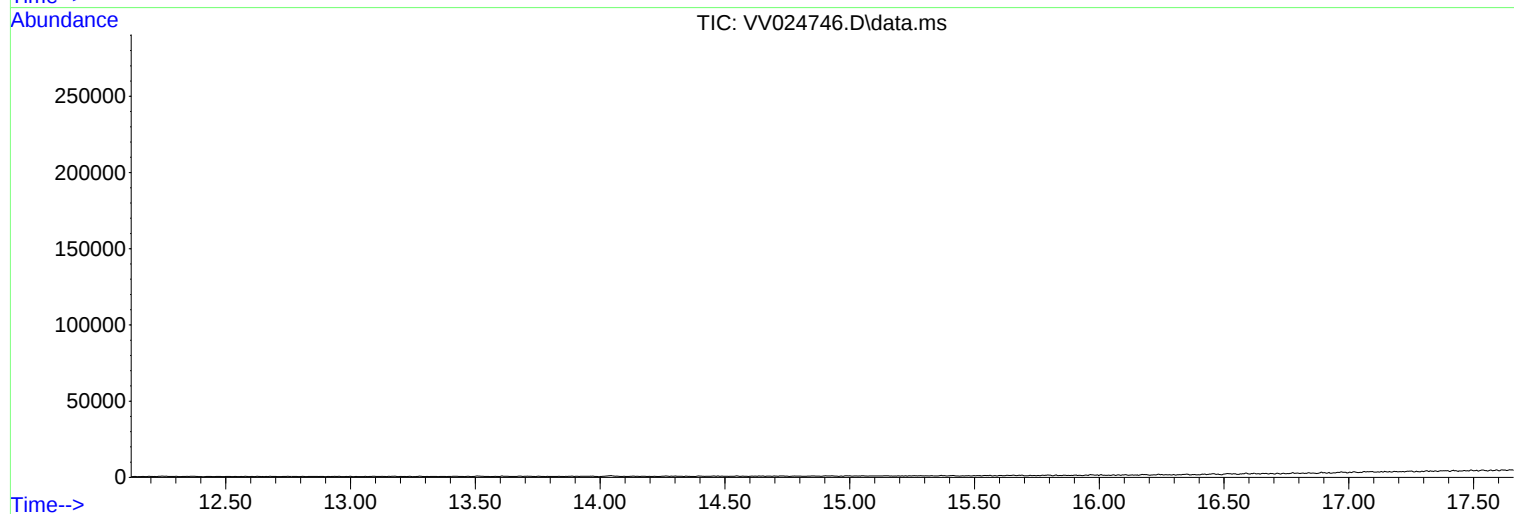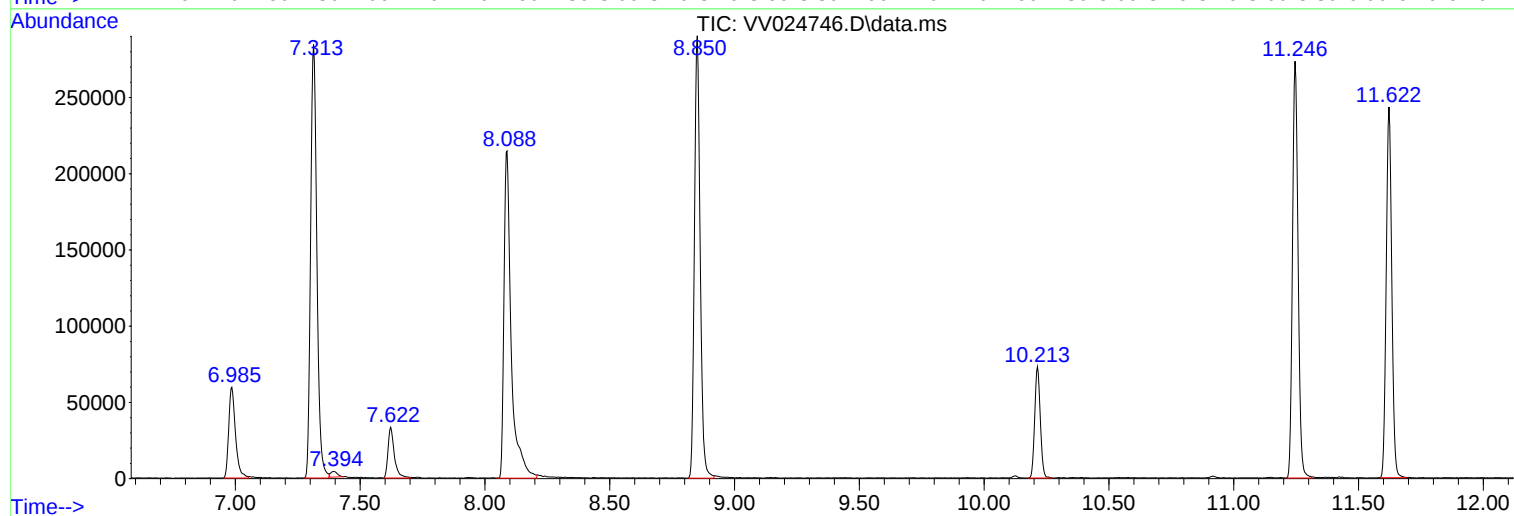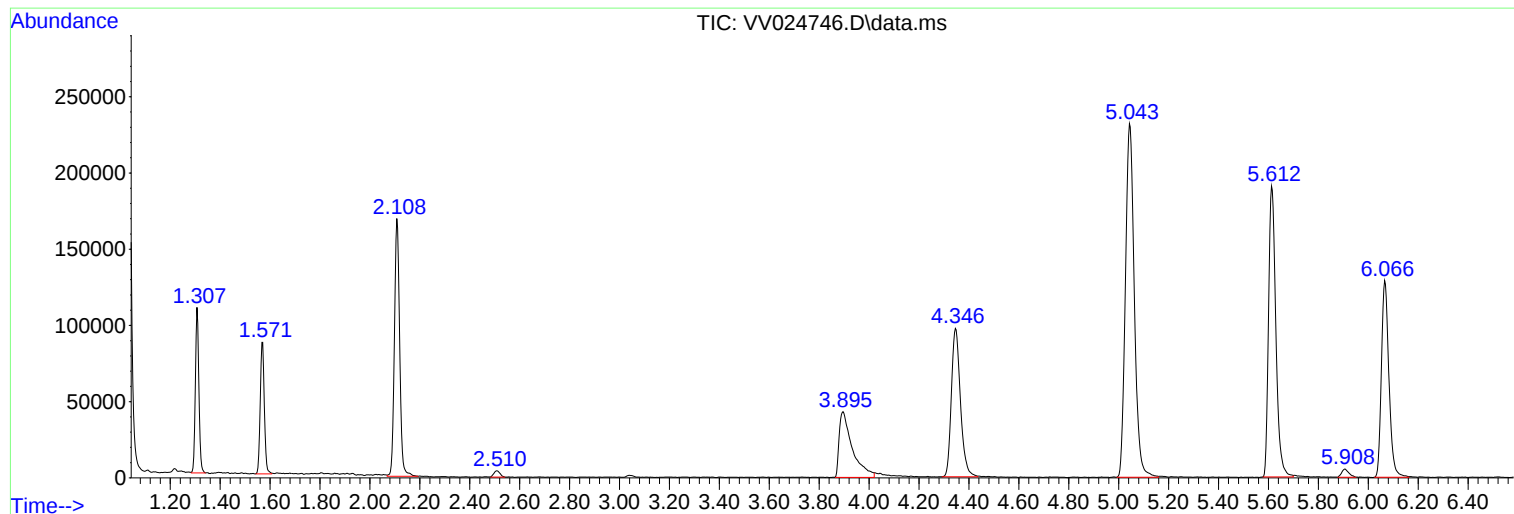

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021822\
Data File : VV024746.D
Acq On : 18 Feb 2022 12:09
Operator : SY/MD
Sample : VV0218WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK308

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021822\
Data File : VV024746.D
Acq On : 18 Feb 2022 12:09
Operator : SY/MD
Sample : VV0218WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK308

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc