

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021822\
 Data File : VV024750.D
 Acq On : 18 Feb 2022 13:55
 Operator : SY/MD
 Sample : N1510-20DL 100X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4M34DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV024750.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	76	84	98	rVB2	138339	143614	24.26%	2.813%
2	1.571	157	165	179	rBV	87885	98459	16.63%	1.929%
3	2.111	322	333	355	rVB	171109	251089	42.42%	4.919%
4	2.773	529	539	554	rVB5	4059	8250	1.39%	0.162%
5	3.912	876	893	929	rBV3	144851	460537	77.80%	9.021%
6	4.352	1011	1030	1062	rBV	100968	254541	43.00%	4.986%
7	5.050	1229	1247	1277	rBV2	237916	591961	100.00%	11.596%
8	5.619	1412	1424	1458	rBV	200557	407580	68.85%	7.984%
9	5.911	1503	1515	1531	rVB5	6464	14011	2.37%	0.274%
10	6.069	1552	1564	1598	rBV	134699	277171	46.82%	5.429%
11	6.989	1837	1850	1872	rBV	61556	112953	19.08%	2.213%
12	7.317	1940	1952	1972	rBV	296650	516294	87.22%	10.114%
13	7.394	1973	1976	1993	rVB4	3996	7459	1.26%	0.146%
14	7.625	2034	2048	2069	rBV	33116	59651	10.08%	1.168%
15	8.088	2182	2192	2231	rBV	236779	466776	78.85%	9.144%
16	8.850	2419	2429	2453	rBV	295496	485149	81.96%	9.503%
17	10.214	2843	2853	2869	rBV	77639	120909	20.43%	2.368%
18	11.249	3163	3175	3191	rBV	286323	438760	74.12%	8.595%
19	11.622	3280	3291	3312	rBV	249418	389817	65.85%	7.636%




Sum of corrected areas: 5104981

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021822\
Data File : VV024750.D
Acq On : 18 Feb 2022 13:55
Operator : SY/MD
Sample : N1510-20DL 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4M34DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

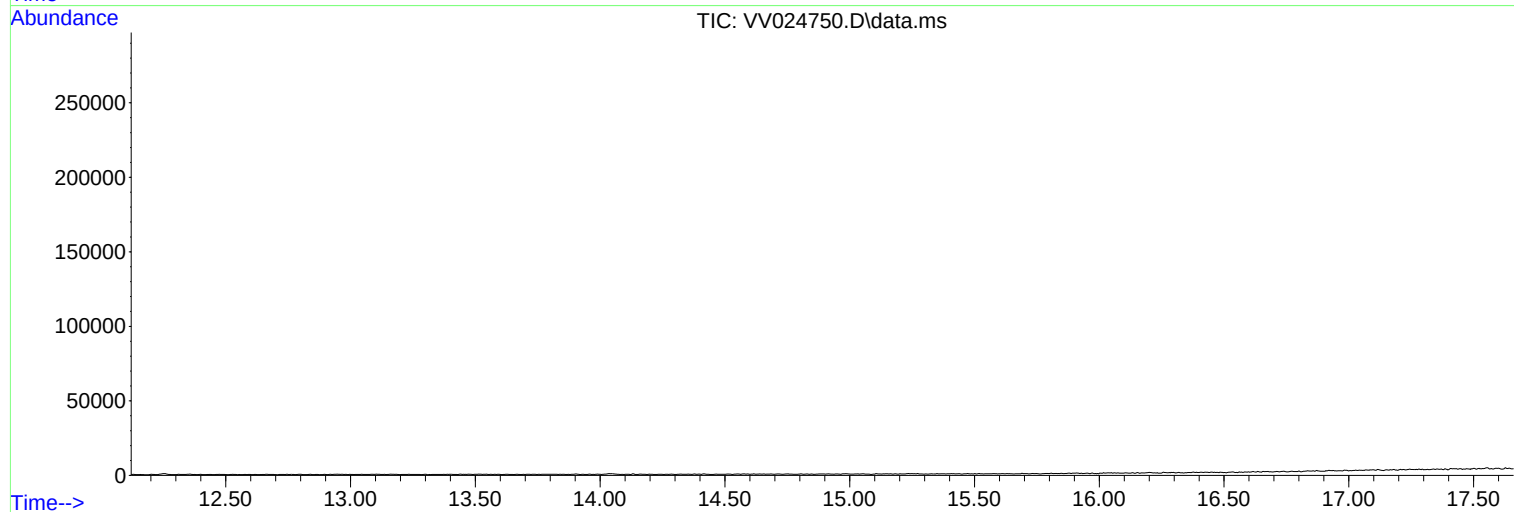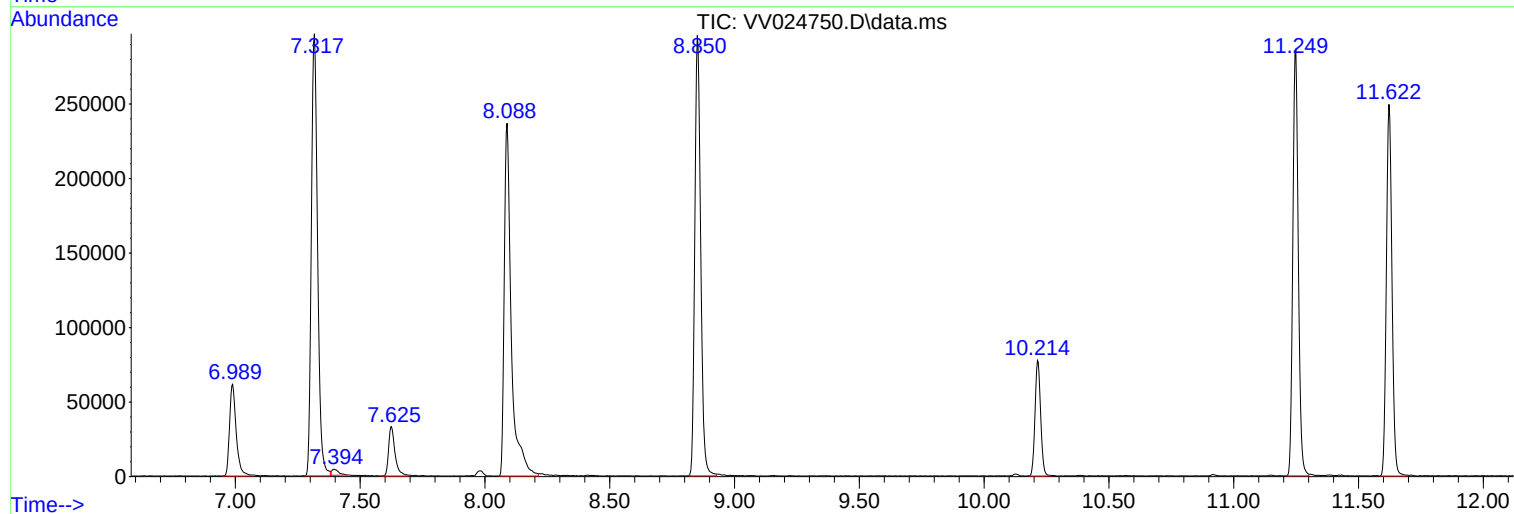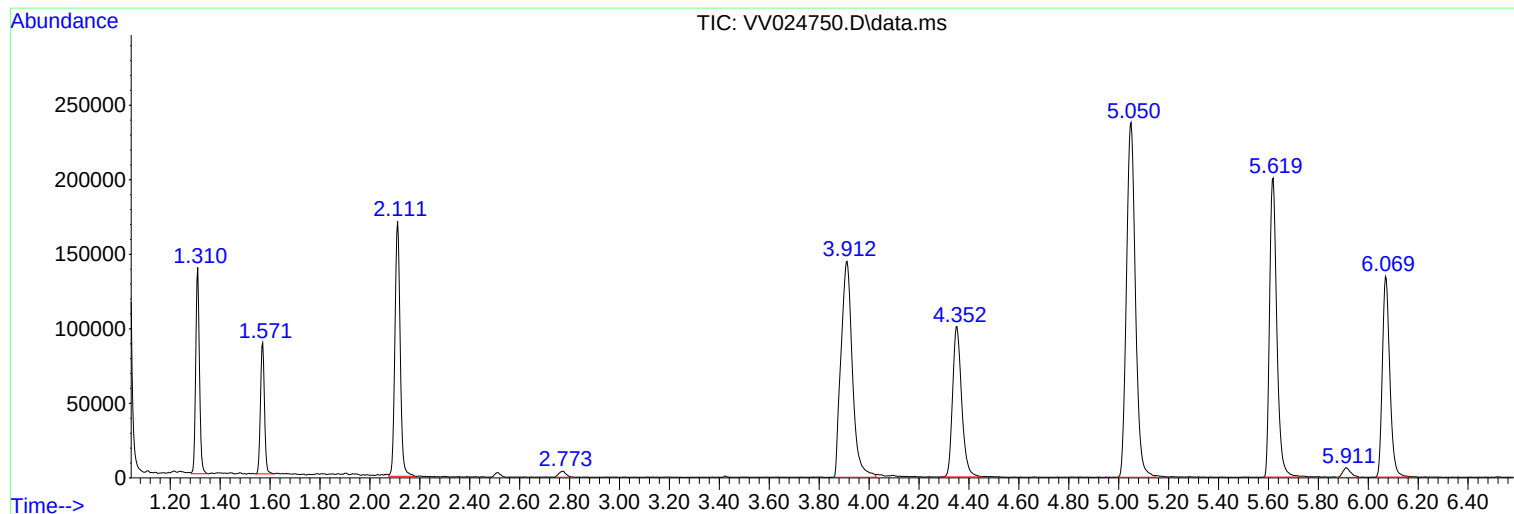

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021822\
Data File : VV024750.D
Acq On : 18 Feb 2022 13:55
Operator : SY/MD
Sample : N1510-20DL 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4M34DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021822\
Data File : VV024750.D
Acq On : 18 Feb 2022 13:55
Operator : SY/MD
Sample : N1510-20DL 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4M34DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc