

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021822\
 Data File : VV024751.D
 Acq On : 18 Feb 2022 14:19
 Operator : SY/MD
 Sample : N1522-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4M72

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV024751.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	101	rVB	97507	99547	17.89%	2.213%
2	1.571	157	165	176	rBV	84248	92131	16.55%	2.048%
3	1.847	248	251	256	rVB	9441	6016	1.08%	0.134%
4	2.111	322	333	349	rBV	159777	229348	41.21%	5.098%
5	3.889	877	886	914	rBV	53216	158657	28.51%	3.527%
6	4.352	1014	1030	1065	rBV	109252	276371	49.66%	6.144%
7	5.050	1230	1247	1278	rBV2	226135	556577	100.00%	12.373%
8	5.619	1410	1424	1456	rBV	183710	371491	66.75%	8.258%
9	5.911	1505	1515	1534	rVB4	6177	14068	2.53%	0.313%
10	6.069	1552	1564	1584	rBV	125601	258948	46.53%	5.756%
11	6.989	1840	1850	1874	rBV	57776	106717	19.17%	2.372%
12	7.317	1939	1952	1969	rBV	276453	483170	86.81%	10.741%
13	7.394	1969	1976	1995	rVB2	11778	25104	4.51%	0.558%
14	7.625	2038	2048	2067	rBV2	31309	55637	10.00%	1.237%
15	8.088	2182	2192	2233	rBV	217083	426388	76.61%	9.478%
16	8.853	2418	2430	2456	rBV	271121	445160	79.98%	9.896%
17	10.217	2841	2854	2868	rBV	68086	107478	19.31%	2.389%
18	11.249	3158	3175	3196	rBV	262983	410855	73.82%	9.133%
19	11.554	3256	3270	3280	rBV7	4438	8007	1.44%	0.178%
20	11.622	3280	3291	3310	rVV	235136	366807	65.90%	8.154%




Sum of corrected areas: 4498477

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021822\
Data File : VV024751.D
Acq On : 18 Feb 2022 14:19
Operator : SY/MD
Sample : N1522-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4M72

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

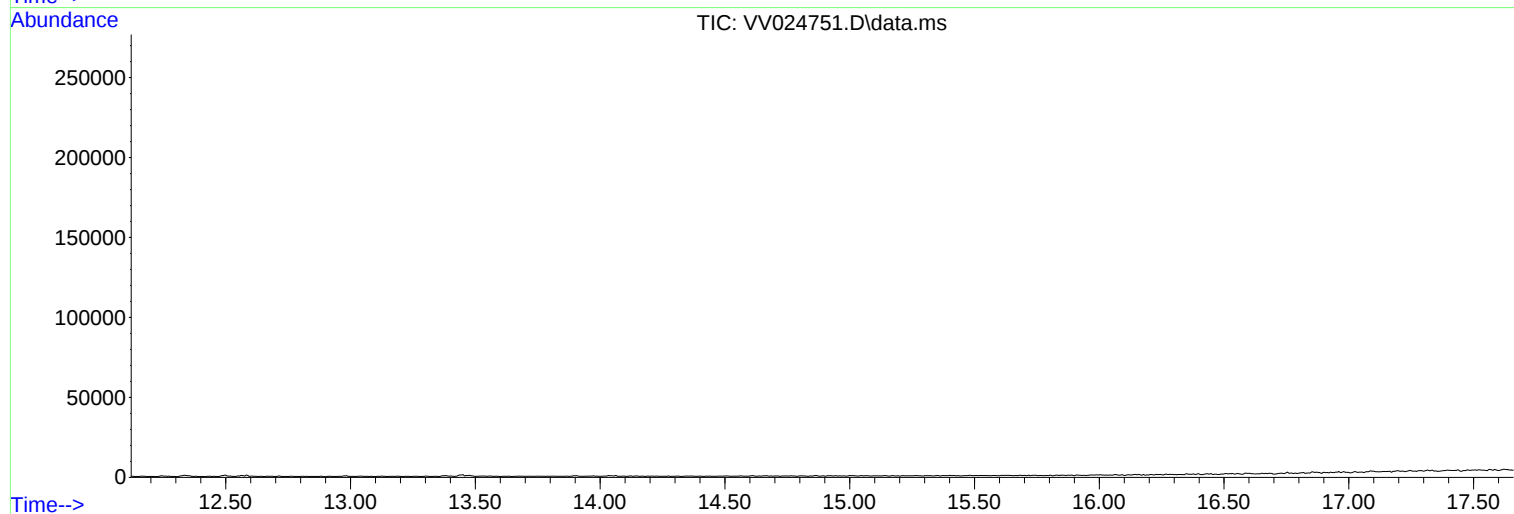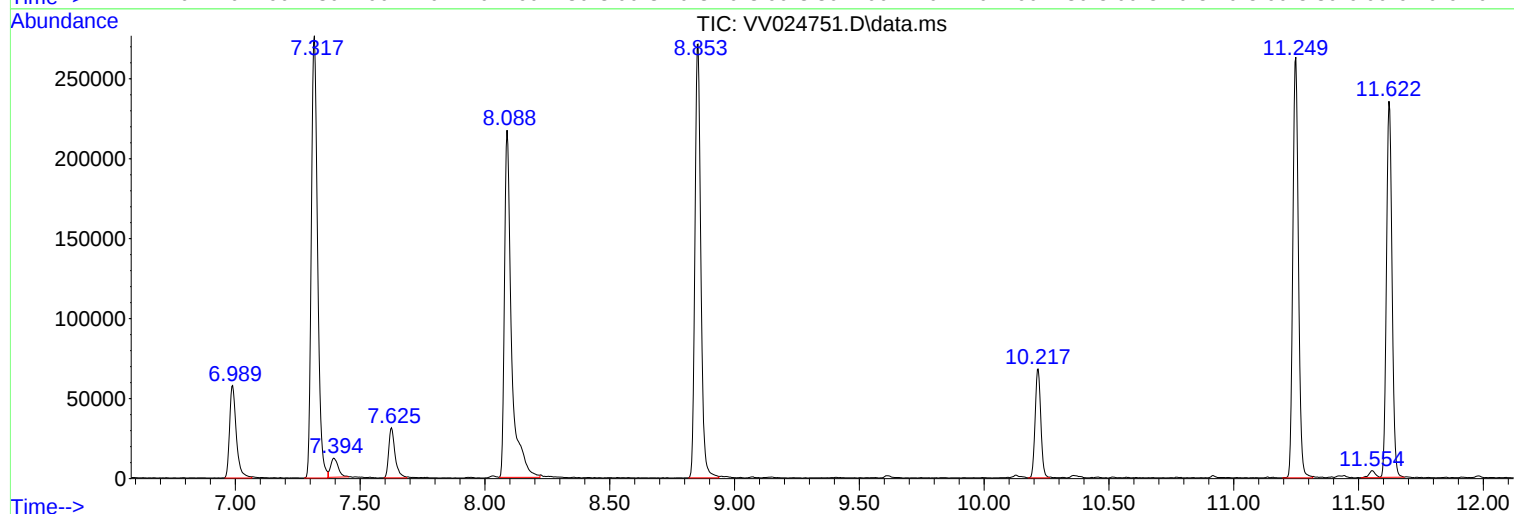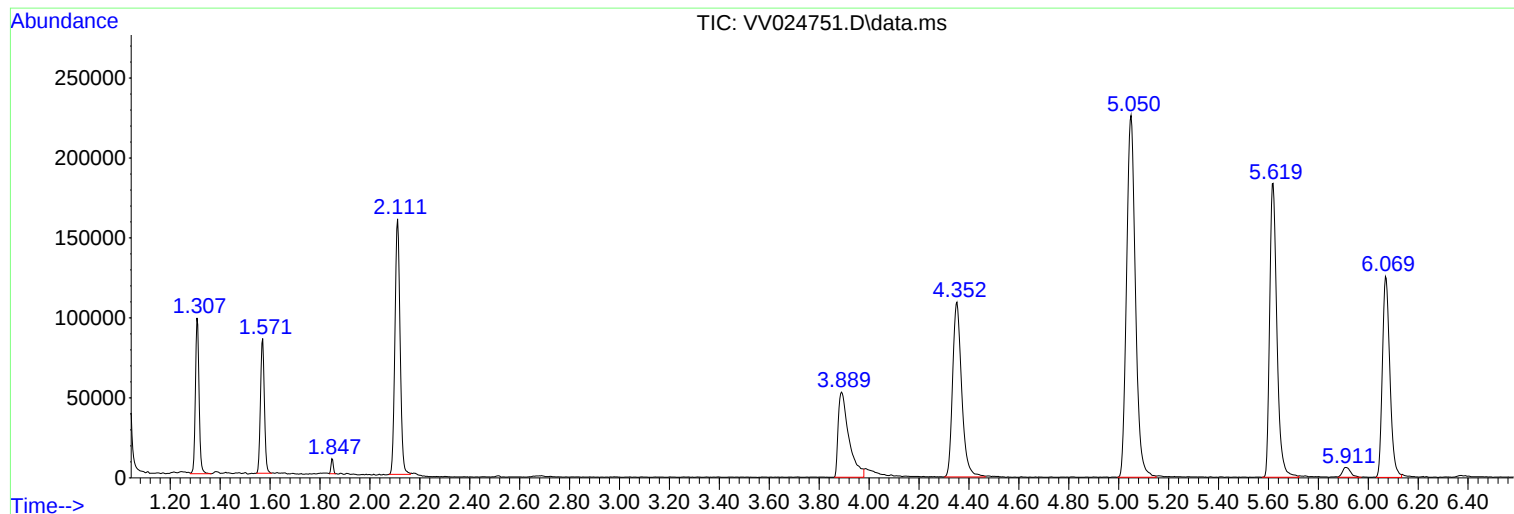

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021822\
Data File : VV024751.D
Acq On : 18 Feb 2022 14:19
Operator : SY/MD
Sample : N1522-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4M72

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021822\
Data File : VV024751.D
Acq On : 18 Feb 2022 14:19
Operator : SY/MD
Sample : N1522-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4M72

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc