

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021822\
 Data File : VV024763.D
 Acq On : 18 Feb 2022 19:01
 Operator : SY/MD
 Sample : N1522-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV024763.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	100	rVB	91515	93963	16.86%	2.110%
2	1.571	156	165	176	rBV	79214	91056	16.33%	2.044%
3	2.111	322	333	355	rBV	149988	218462	39.19%	4.905%
4	3.892	877	887	927	rBV	54825	171403	30.75%	3.848%
5	4.352	1014	1030	1056	rBV2	95549	243196	43.63%	5.460%
6	5.047	1230	1246	1275	rBV2	223594	557440	100.00%	12.515%
7	5.619	1411	1424	1455	rBV	163318	332707	59.68%	7.470%
8	5.915	1505	1516	1532	rVB3	5048	10032	1.80%	0.225%
9	6.069	1551	1564	1588	rBV2	125303	257403	46.18%	5.779%
10	6.989	1839	1850	1872	rBV2	58222	108795	19.52%	2.443%
11	7.317	1940	1952	1970	rBV	275654	476304	85.44%	10.694%
12	7.400	1971	1978	1996	rVB2	5304	11417	2.05%	0.256%
13	7.625	2039	2048	2071	rBV	32542	57869	10.38%	1.299%
14	8.088	2180	2192	2235	rBV	233942	457684	82.10%	10.275%
15	8.850	2418	2429	2448	rBV	260814	425136	76.27%	9.545%
16	10.214	2843	2853	2869	rBV2	74888	117275	21.04%	2.633%
17	11.249	3164	3175	3198	rBV	280480	435909	78.20%	9.787%
18	11.622	3280	3291	3317	rBV	244296	377247	67.67%	8.470%
19	14.844	4282	4293	4301	rBV3	7154	10837	1.94%	0.243%




Sum of corrected areas: 4454135

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021822\
Data File : VV024763.D
Acq On : 18 Feb 2022 19:01
Operator : SY/MD
Sample : N1522-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

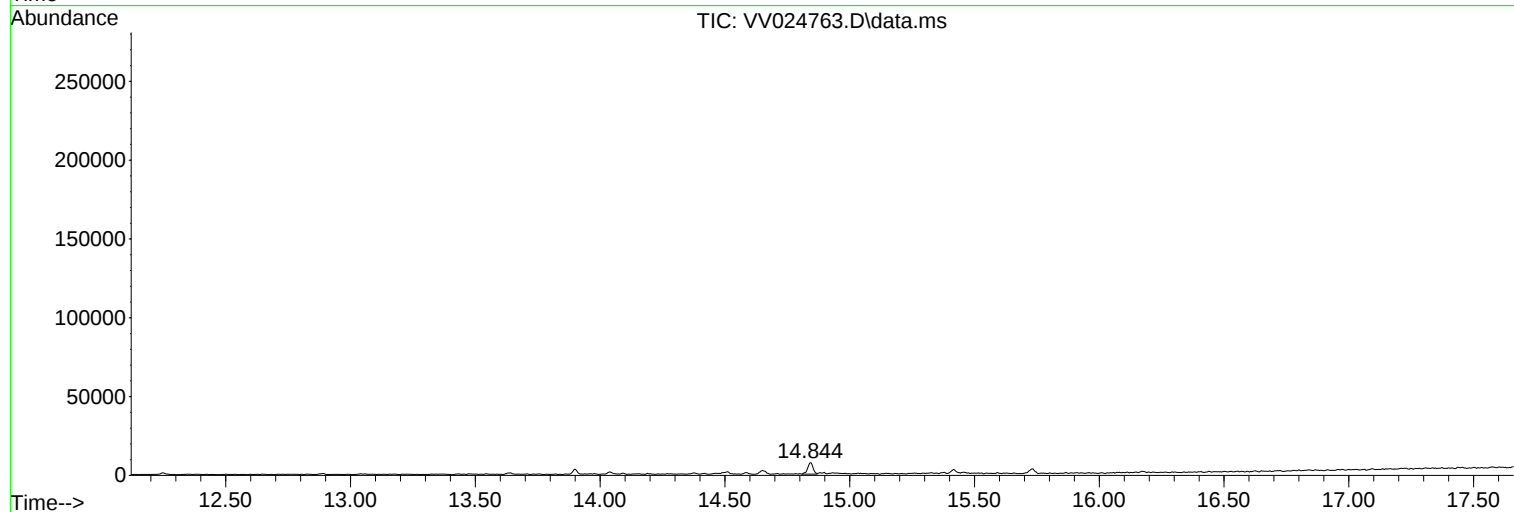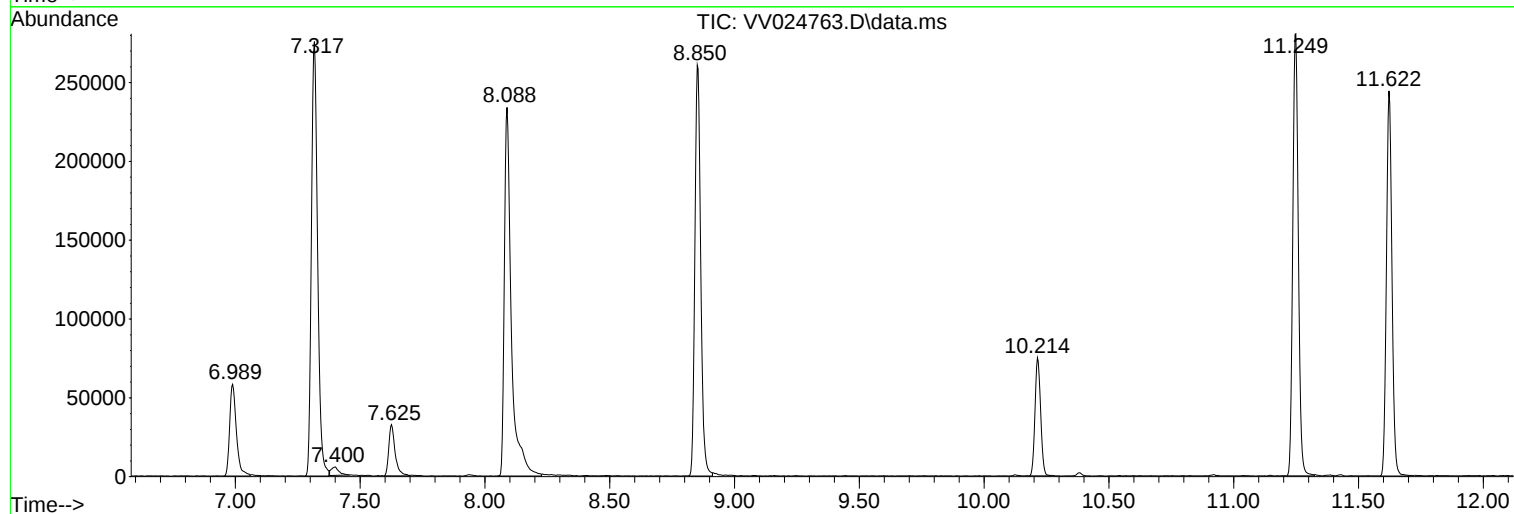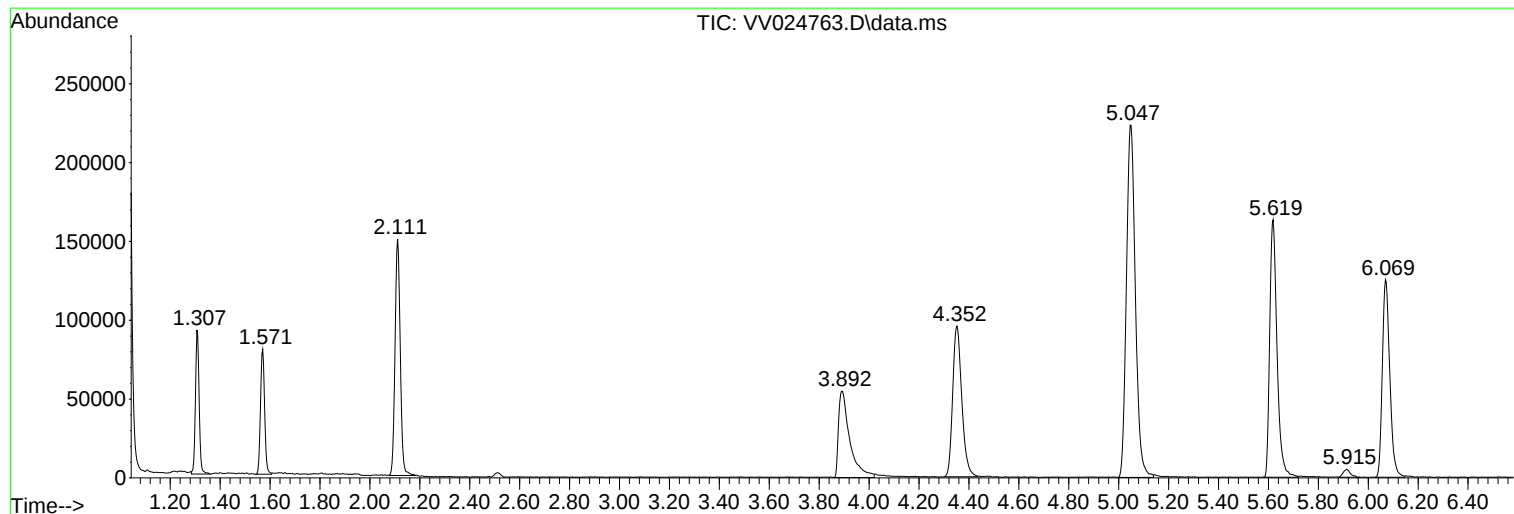

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021822\
Data File : VV024763.D
Acq On : 18 Feb 2022 19:01
Operator : SY/MD
Sample : N1522-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021822\
Data File : VV024763.D
Acq On : 18 Feb 2022 19:01
Operator : SY/MD
Sample : N1522-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
