

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021822\
 Data File : VV024764.D
 Acq On : 18 Feb 2022 19:24
 Operator : SY/MD
 Sample : N1510-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4M30

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV024764.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	76	84	92	rBV	89929	91499	16.27%	2.010%
2	1.571	157	165	178	rVB	83692	92821	16.50%	2.039%
3	2.111	323	333	349	rBV	150543	216923	38.57%	4.766%
4	3.892	874	887	925	rBV	54166	170205	30.26%	3.739%
5	4.352	1010	1030	1069	rBV	92321	242369	43.09%	5.325%
6	5.050	1230	1247	1279	rBV2	225571	562441	100.00%	12.357%
7	5.616	1412	1423	1448	rBV	192299	386081	68.64%	8.482%
8	5.918	1506	1517	1530	rVB7	4763	9432	1.68%	0.207%
9	6.069	1550	1564	1588	rBV	127616	262318	46.64%	5.763%
10	6.989	1839	1850	1873	rBV	57467	108430	19.28%	2.382%
11	7.317	1938	1952	1971	rBV	273959	479288	85.22%	10.530%
12	7.397	1971	1977	1989	rVB3	3712	7643	1.36%	0.168%
13	7.625	2037	2048	2072	rBV	31230	57405	10.21%	1.261%
14	8.088	2182	2192	2230	rBV	242935	466086	82.87%	10.240%
15	8.850	2417	2429	2460	rBV	280480	461652	82.08%	10.142%
16	10.214	2843	2853	2868	rBV	77074	120382	21.40%	2.645%
17	11.246	3163	3174	3192	rBV	277905	428632	76.21%	9.417%
18	11.622	3280	3291	3320	rVB	239819	379625	67.50%	8.340%
19	14.844	4285	4293	4301	rVB3	6231	8506	1.51%	0.187%




Sum of corrected areas: 4551738

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021822\
Data File : VV024764.D
Acq On : 18 Feb 2022 19:24
Operator : SY/MD
Sample : N1510-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4M30

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

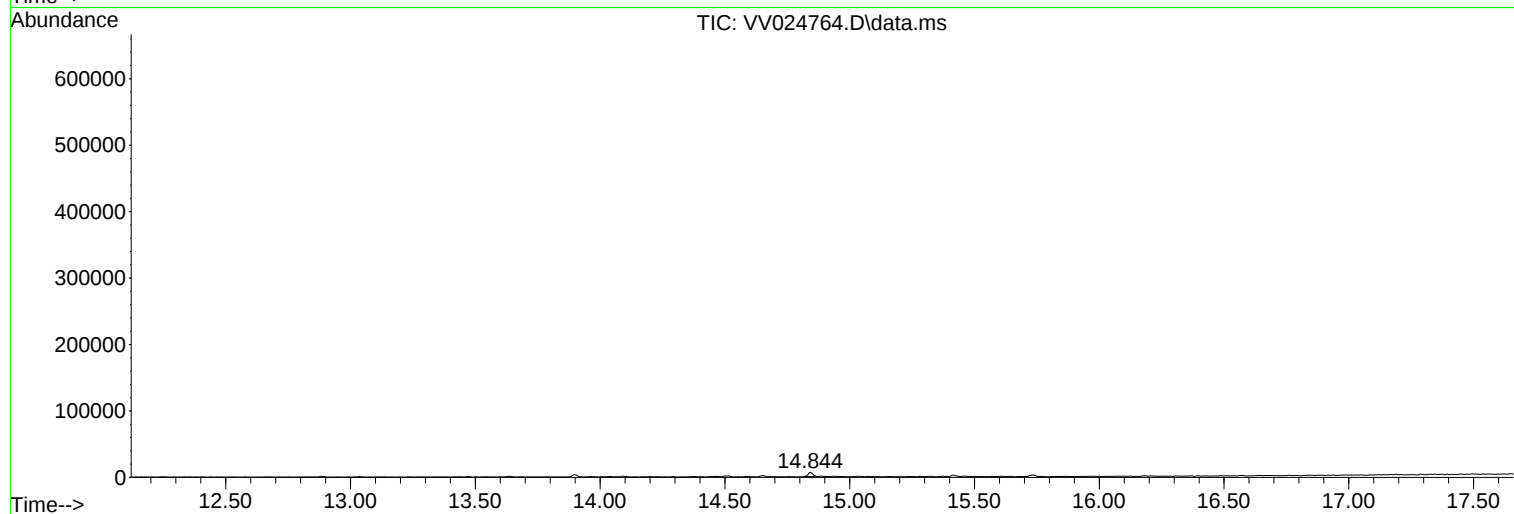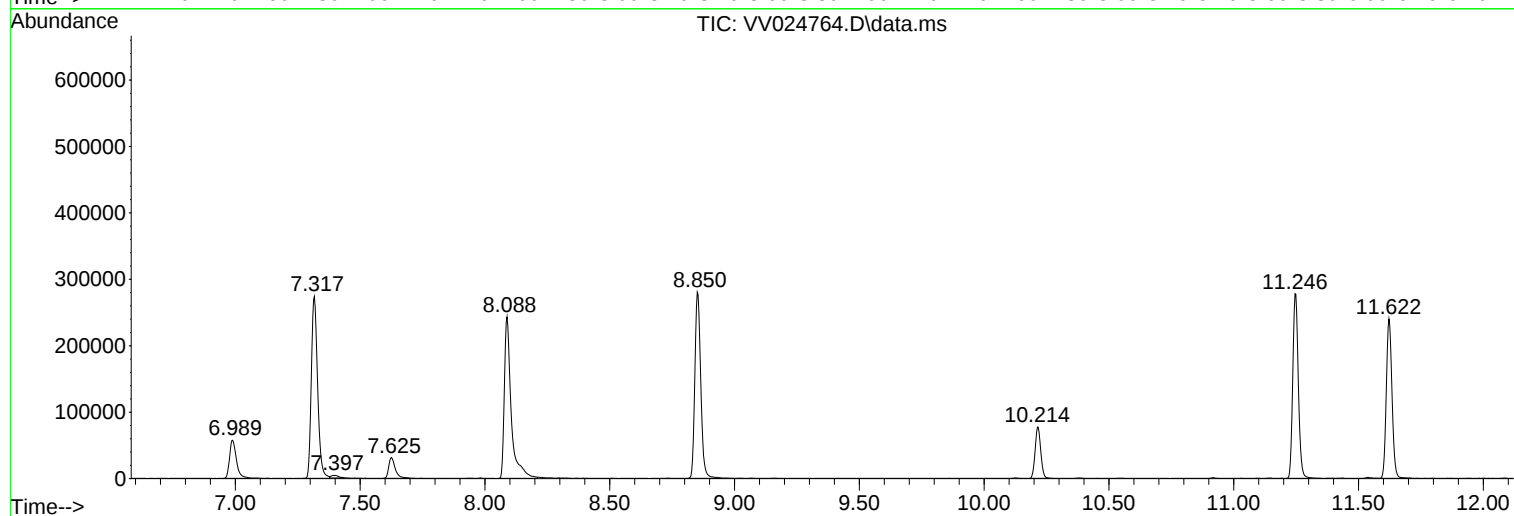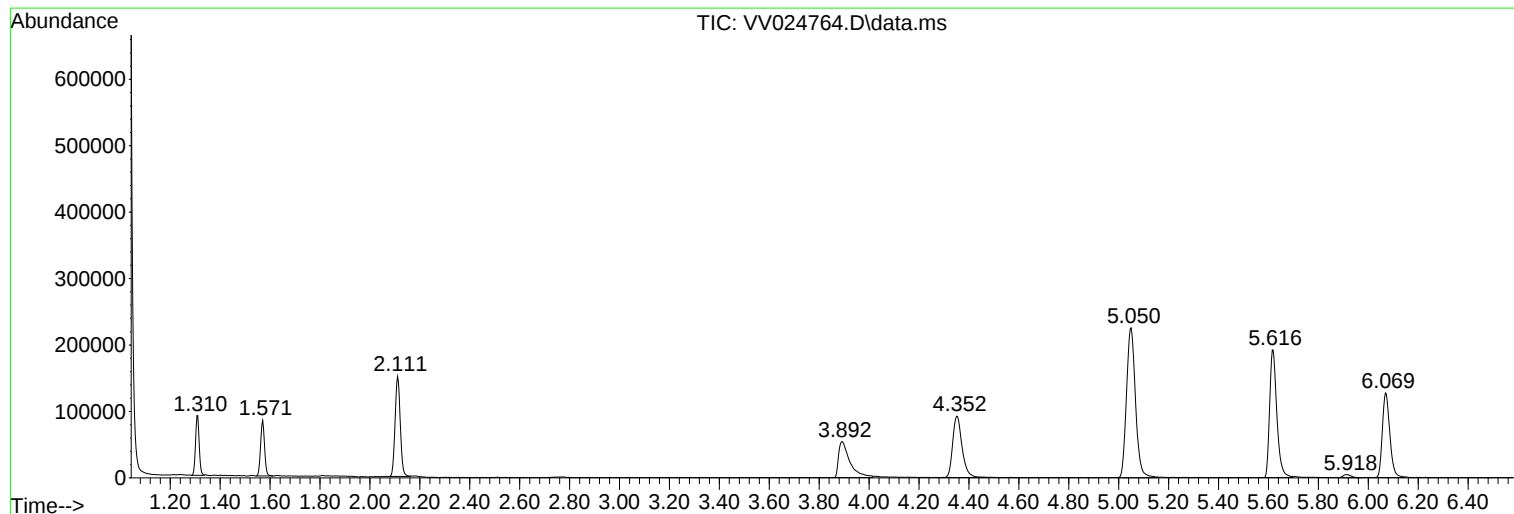

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021822\
Data File : VV024764.D
Acq On : 18 Feb 2022 19:24
Operator : SY/MD
Sample : N1510-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4M30

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021822\
Data File : VV024764.D
Acq On : 18 Feb 2022 19:24
Operator : SY/MD
Sample : N1510-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4M30

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc