
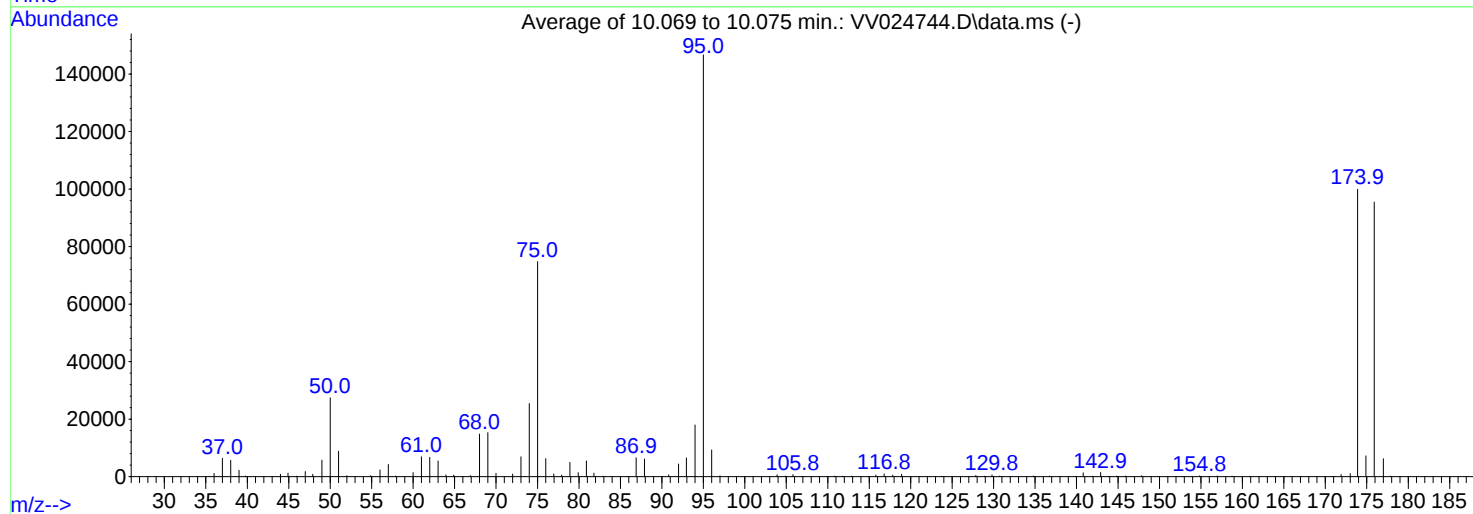


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021822\
 Data File : VV024744.D
 Acq On : 18 Feb 2022 08:48
 Operator : SY/MD
 Sample : BFB273
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB273

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Tue Feb 22 03:27:30 2022

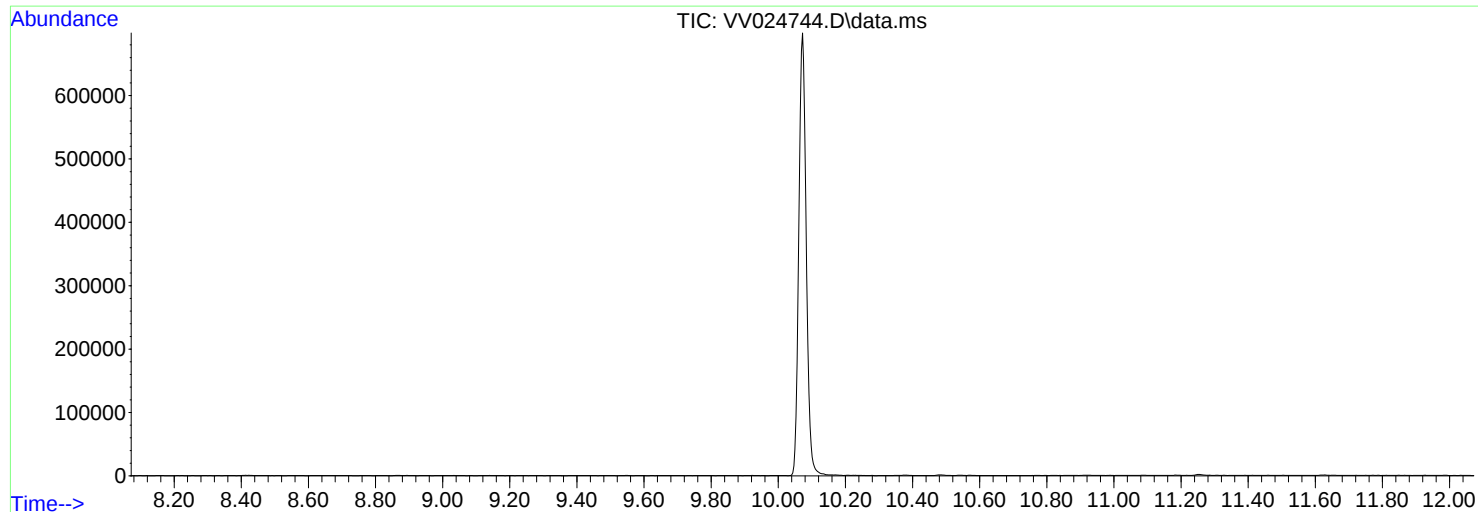

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	27453	PASS
75	95	30	80	51.0	74757	PASS
95	95	100	100	100.0	146667	PASS
96	95	5	9	6.3	9293	PASS
173	174	0.00	2	1.1	1071	PASS
174	95	50	120	68.1	99939	PASS
175	174	5	9	7.2	7241	PASS
176	174	95	105	95.5	95451	PASS
177	176	5	10	6.6	6257	PASS

m/z	Abundance
44.00	332.0

Instrument :
MSVOA_V
ClientSampleId :
BFB273

m/z	Abundance
36.00	1104.0
37.00	6617.0
38.00	5722.0
39.00	2284.0
39.80	280.0
43.00	148.0
44.00	1212.0
44.90	1239.0
46.00	167.0
47.00	1729.0
47.90	837.0
49.00	5757.0
50.00	27768.0
51.00	9063.0
52.00	362.0
54.80	340.0
56.00	2380.0
57.00	4168.0
57.90	216.0
60.00	1377.0
61.00	7073.0
62.00	6844.0
63.00	5441.0
64.00	662.0
64.90	554.0
66.90	369.0
68.00	14968.0
69.00	15476.0
70.00	1225.0
72.00	907.0
73.00	7194.0
74.00	25456.0
75.00	75328.0
76.00	6415.0
77.00	927.0
78.00	560.0
78.90	4935.0
79.90	1359.0
80.90	5513.0
81.80	1275.0
83.00	183.0
85.80	183.0
86.90	6510.0
87.90	6020.0
90.80	612.0
92.00	4258.0
92.90	6472.0
94.00	17824.0
95.00	145664.0
96.00	9450.0
97.00	287.0
103.90	630.0
104.90	179.0
105.80	736.0
110.90	224.0
111.80	171.0
112.90	183.0
114.90	138.0
115.80	532.0
116.80	907.0
117.90	502.0
118.90	836.0
123.70	117.0
127.90	427.0
128.90	197.0
129.80	553.0
130.70	184.0
134.80	252.0
136.70	203.0
139.90	126.0
140.80	1362.0
141.90	171.0
142.90	1502.0
143.90	134.0
144.90	273.0
145.90	224.0
146.90	104.0
147.80	305.0
154.80	332.0
157.00	218.0
158.70	159.0
160.90	165.0
171.90	703.0
173.00	967.0
173.90	97176.0
174.90	7319.0
175.90	92880.0
177.00	6121.0
177.90	208.0

Instrument :
MSVOA_V
ClientSampleId :
BFB273

m/z	Abundance
36.00	1184.0
37.00	6565.0
38.00	5842.0
39.00	2314.0
39.80	260.0
43.00	121.0
44.00	1186.0
44.90	1314.0
45.90	151.0
47.00	1882.0
47.90	845.0
49.00	5902.0
50.00	28472.0
51.00	9139.0
52.00	363.0
54.80	350.0
56.00	2375.0
57.00	4443.0
57.90	224.0
60.00	1409.0
61.00	7165.0
62.00	6896.0
63.00	5633.0
64.00	603.0
64.90	552.0
65.90	119.0
66.90	365.0
68.00	15343.0
69.00	15846.0
70.00	1220.0
72.00	916.0
73.00	7182.0
74.00	26224.0
75.00	77208.0
76.00	6532.0
76.90	952.0
77.90	586.0
78.90	5098.0
79.90	1393.0
80.90	5686.0
81.80	1289.0
82.90	160.0
85.80	154.0
86.90	6823.0
87.90	6410.0
90.80	648.0
92.00	4586.0
92.90	6727.0
94.00	18696.0
95.00	152192.0
96.00	9569.0
97.00	312.0
103.90	671.0
104.90	213.0
105.80	734.0
106.80	112.0
107.00	106.0
110.80	230.0
111.80	190.0
112.90	160.0
114.90	124.0
115.80	586.0
116.80	974.0
117.80	546.0
118.90	903.0
123.70	128.0
127.80	462.0
128.90	198.0
129.80	645.0
130.70	218.0
134.80	252.0
136.80	204.0
139.90	141.0
140.80	1414.0
141.90	207.0
142.90	1508.0
143.80	131.0
144.90	253.0
145.90	245.0
147.80	320.0
154.00	101.0
154.80	293.0
157.00	222.0
158.80	159.0
160.90	157.0
171.90	746.0
173.00	1101.0
173.90	103656.0
174.90	7445.0
175.90	98832.0
177.00	6504.0
177.90	191.0

Instrument :
MSVOA_V
ClientSampleId :
BFB273

m/z	Abundance
36.00	1114.0
37.00	5788.0
38.00	5469.0
39.00	2089.0
39.80	210.0
43.00	106.0
44.00	1067.0
44.90	1175.0
45.90	145.0
47.00	1809.0
47.90	785.0
49.00	5512.0
50.00	26120.0
51.00	8282.0
52.00	345.0
54.90	361.0
56.00	2222.0
57.00	4167.0
57.90	204.0
60.00	1335.0
61.00	6540.0
62.00	6476.0
63.00	5276.0
63.90	534.0
64.90	529.0
65.90	114.0
66.90	328.0
68.00	14095.0
69.00	14568.0
70.00	1119.0
72.00	868.0
73.00	6315.0
74.00	24568.0
75.00	71736.0
76.00	6009.0
77.00	899.0
77.80	608.0
78.90	4848.0
79.90	1373.0
80.90	5214.0
81.80	1135.0
82.80	121.0
86.00	180.0
86.90	6458.0
87.90	5945.0
90.80	606.0
92.00	4357.0
93.00	6340.0
94.00	17352.0
95.00	142144.0
96.00	8860.0
97.00	319.0
103.90	681.0
104.90	219.0
105.80	656.0
106.80	113.0
107.00	104.0
109.90	104.0
110.80	193.0
111.80	176.0
112.80	131.0
114.80	119.0
115.80	614.0
116.80	945.0
117.80	609.0
118.90	814.0
123.80	121.0
127.80	494.0
128.90	178.0
129.80	657.0
130.80	206.0
134.80	251.0
136.80	200.0
139.90	127.0
140.80	1311.0
141.90	187.0
142.90	1397.0
143.80	122.0
144.80	205.0
145.90	208.0
147.90	330.0
149.80	116.0
152.80	111.0
154.90	268.0
156.90	199.0
158.70	143.0
160.90	135.0
170.70	105.0
171.10	104.0
171.90	665.0
173.00	1145.0
173.90	98984.0

Instrument :
MSVOA_V
ClientSampleId :
BFB273

174.90	6958.0
175.90	94640.0
177.00	6147.0
177.90	146.0

Instrument :
MSVOA_V
ClientSampleId :
BFB273