

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022024\
 Data File : VV034263.D
 Acq On : 20 Feb 2024 12:27
 Operator : SY/MD
 Sample : P1501-18
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E10B6

Quant Time: Feb 21 01:43:12 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Feb 21 01:41:15 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	73732	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	66497	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	33607	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	21191	3.711	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	74.200%
7) Chloroethane-d5	1.535	69	19777	3.954	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	79.000%
11) 1,1-Dichloroethene-d2	2.060	65	10658	3.870	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	77.400%
20) 2-Butanone-d5	3.812	46	37096	38.680	ug/L	-0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	77.360%
24) Chloroform-d	4.249	84	44379	4.277	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.600%
26) 1,2-Dichloroethane-d4	4.944	65	22464	4.633	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.600%
32) Benzene-d6	4.960	84	83068	4.164	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	83.200%
36) 1,2-Dichloropropane-d6	5.989	67	22516	4.037	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	80.800%
41) Toluene-d8	7.243	98	77697	4.237	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.800%
43) trans-1,3-Dichloroprop...	7.564	79	7460	3.543	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	70.800%
46) 2-Hexanone-d5	8.027	63	28584	38.024	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	76.040%
56) 1,1,2,2-Tetrachloroeth...	10.152	84	14063	4.160	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	83.200%
66) 1,2-Dichlorobenzene-d4	11.561	152	26506	4.337	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	86.800%
Target Compounds						
					Qvalue	
25) Chloroform	4.275	83	3383	0.347	ug/L	96
42) Toluene	7.326	91	5976	0.280	ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022024\
Data File : VV034263.D
Acq On : 20 Feb 2024 12:27
Operator : SY/MD
Sample : P1501-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E10B6

Quant Time: Feb 21 01:43:12 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Feb 21 01:41:15 2024
Response via : Initial Calibration




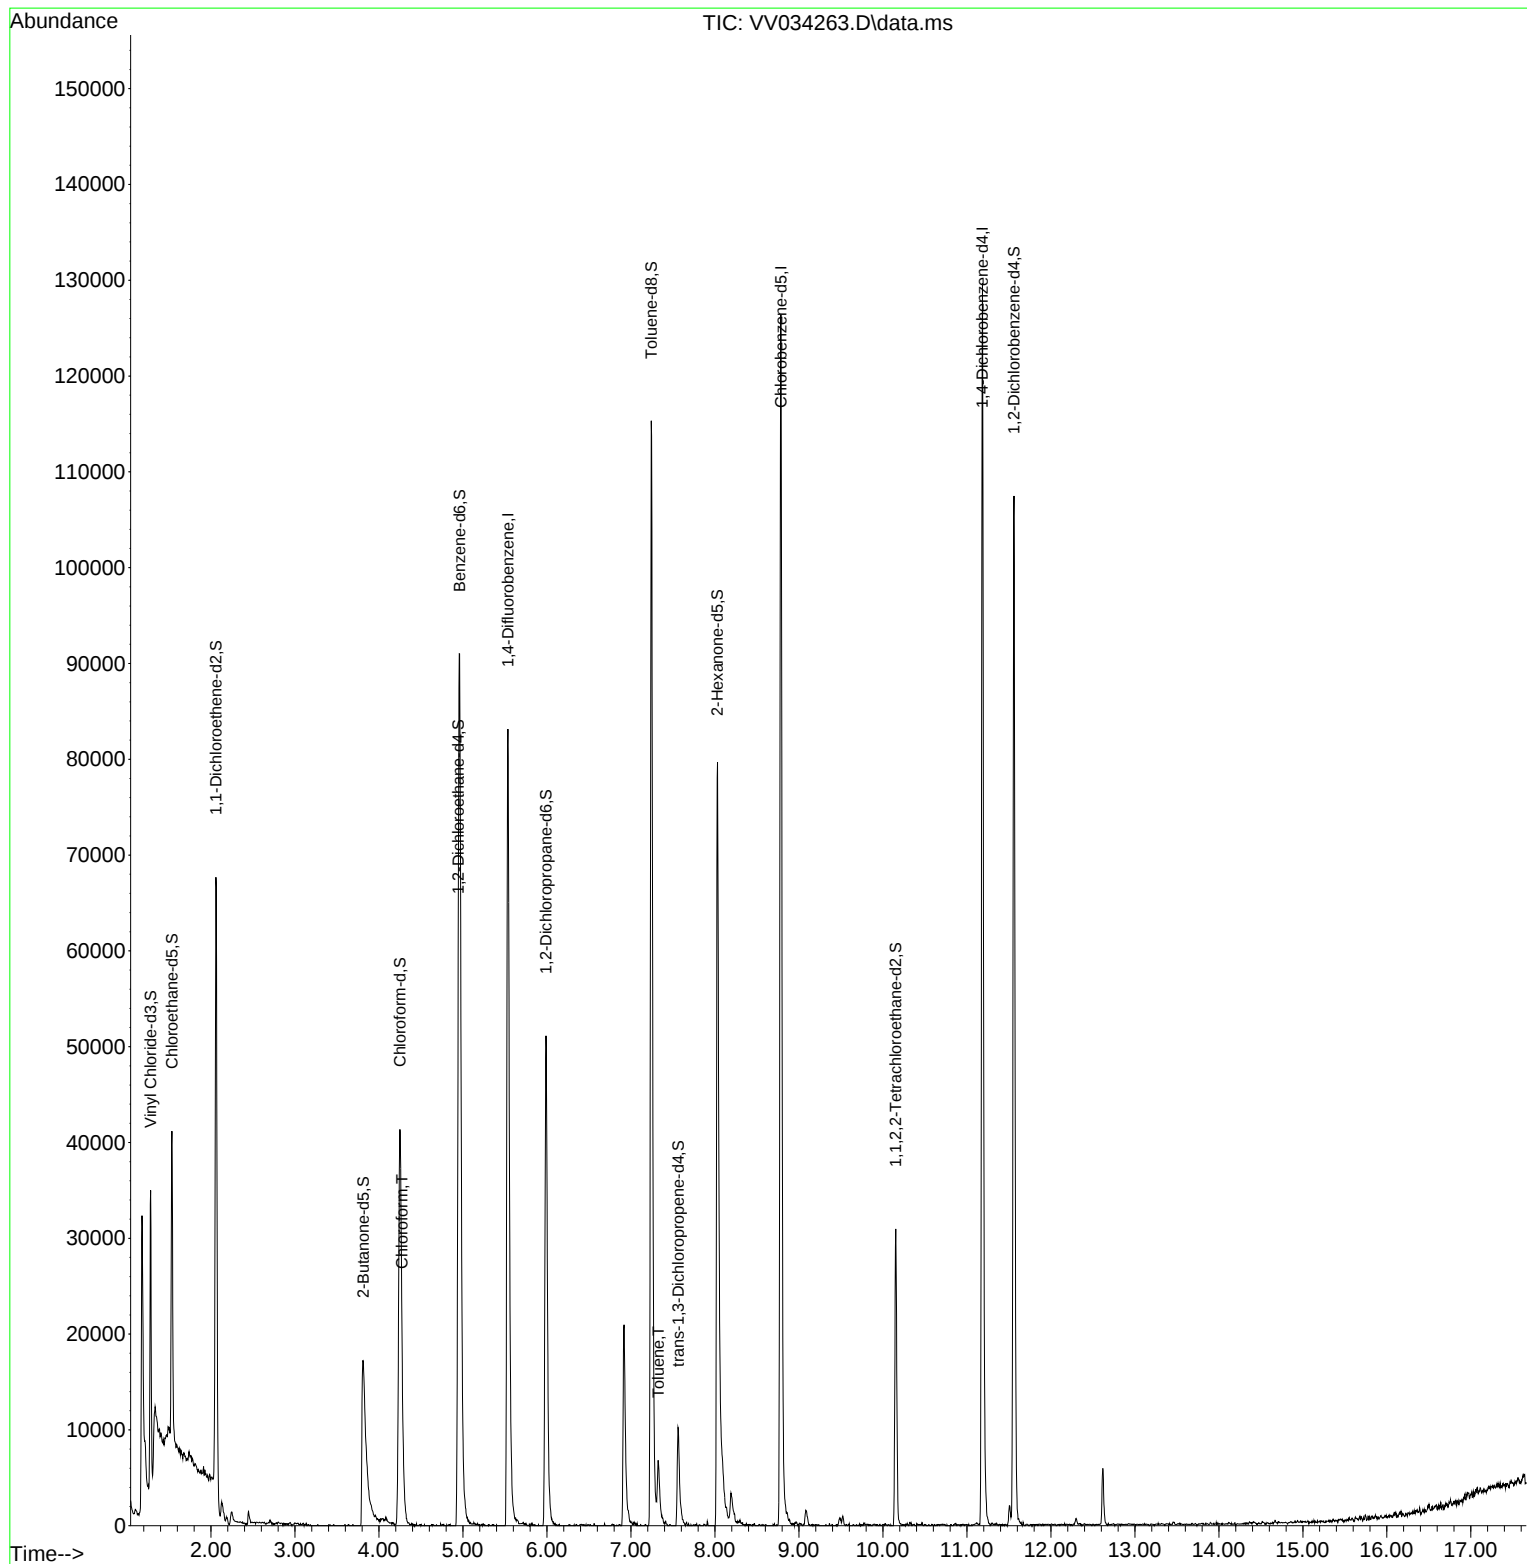


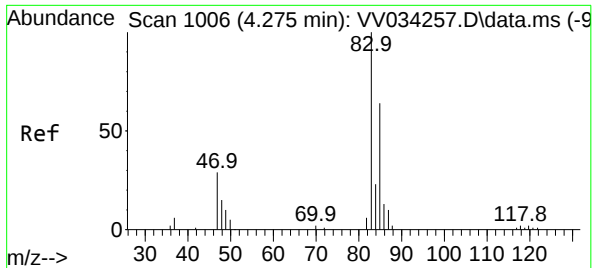

#25
Chloroform
Concen: 0.347 ug/L
RT: 4.275 min Scan# 1006
Delta R.T. -0.000 min
Lab File: VV034263.D
Acq: 20 Feb 2024 12:27

Instrument :
MSVOA_V
ClientSampleId :
E10B6

Tgt Ion: 83 Resp: 3383
Ion Ratio Lower Upper
83 100
85 64.7 47.5 88.1

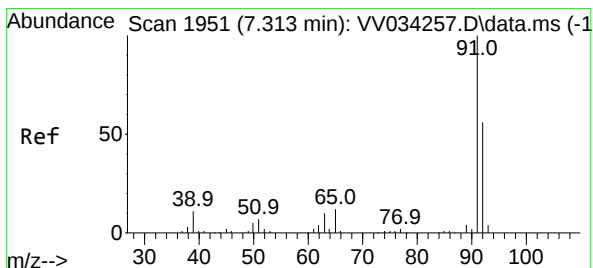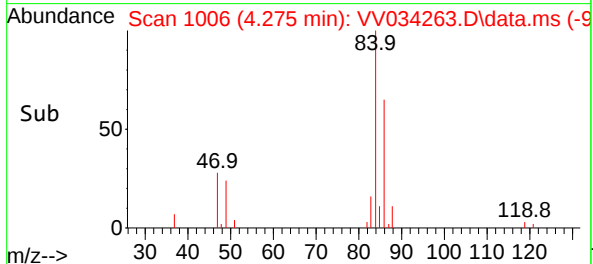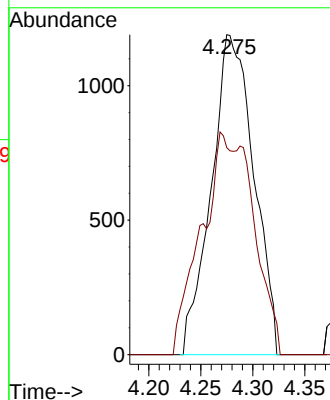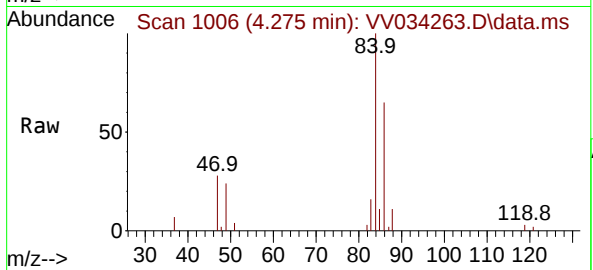

#42
Toluene
Concen: 0.280 ug/L
RT: 7.326 min Scan# 1955
Delta R.T. 0.013 min
Lab File: VV034263.D
Acq: 20 Feb 2024 12:27

Tgt Ion: 91 Resp: 5976
Ion Ratio Lower Upper
91 100
92 53.4 42.1 78.3

