

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022024\
 Data File : VV034279.D
 Acq On : 20 Feb 2024 18:58
 Operator : SY/MD
 Sample : P1498-17 500X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB7

Quant Time: Feb 21 01:47:01 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Feb 21 01:41:15 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	61321	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	56594	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	25831	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	19083	4.018	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	80.400%
7) Chloroethane-d5	1.536	69	17883	4.299	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	86.000%
11) 1,1-Dichloroethene-d2	2.060	65	9940	4.340	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	86.800%
20) 2-Butanone-d5	3.828	46	42832	53.701	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	107.400%
24) Chloroform-d	4.252	84	43745	5.069	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.400%
26) 1,2-Dichloroethane-d4	4.947	65	23571	5.845	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	116.800%
32) Benzene-d6	4.963	84	79640	4.690	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.800%
36) 1,2-Dichloropropane-d6	5.992	67	22917	4.828	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.600%
41) Toluene-d8	7.246	98	69827	4.475	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.400%
43) trans-1,3-Dichloroprop...	7.561	79	8044	4.488	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	89.800%
46) 2-Hexanone-d5	8.030	63	34636	54.137	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	108.280%
56) 1,1,2,2-Tetrachloroeth...	10.156	84	15890	5.522	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	110.400%
66) 1,2-Dichlorobenzene-d4	11.561	152	25716	5.474	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	109.400%
Target Compounds						Qvalue
16) Methylene chloride	2.449	84	949	0.231	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022024\
Data File : VV034279.D
Acq On : 20 Feb 2024 18:58
Operator : SY/MD
Sample : P1498-17 500X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB7


Quant Time: Feb 21 01:47:01 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Feb 21 01:41:15 2024
Response via : Initial Calibration

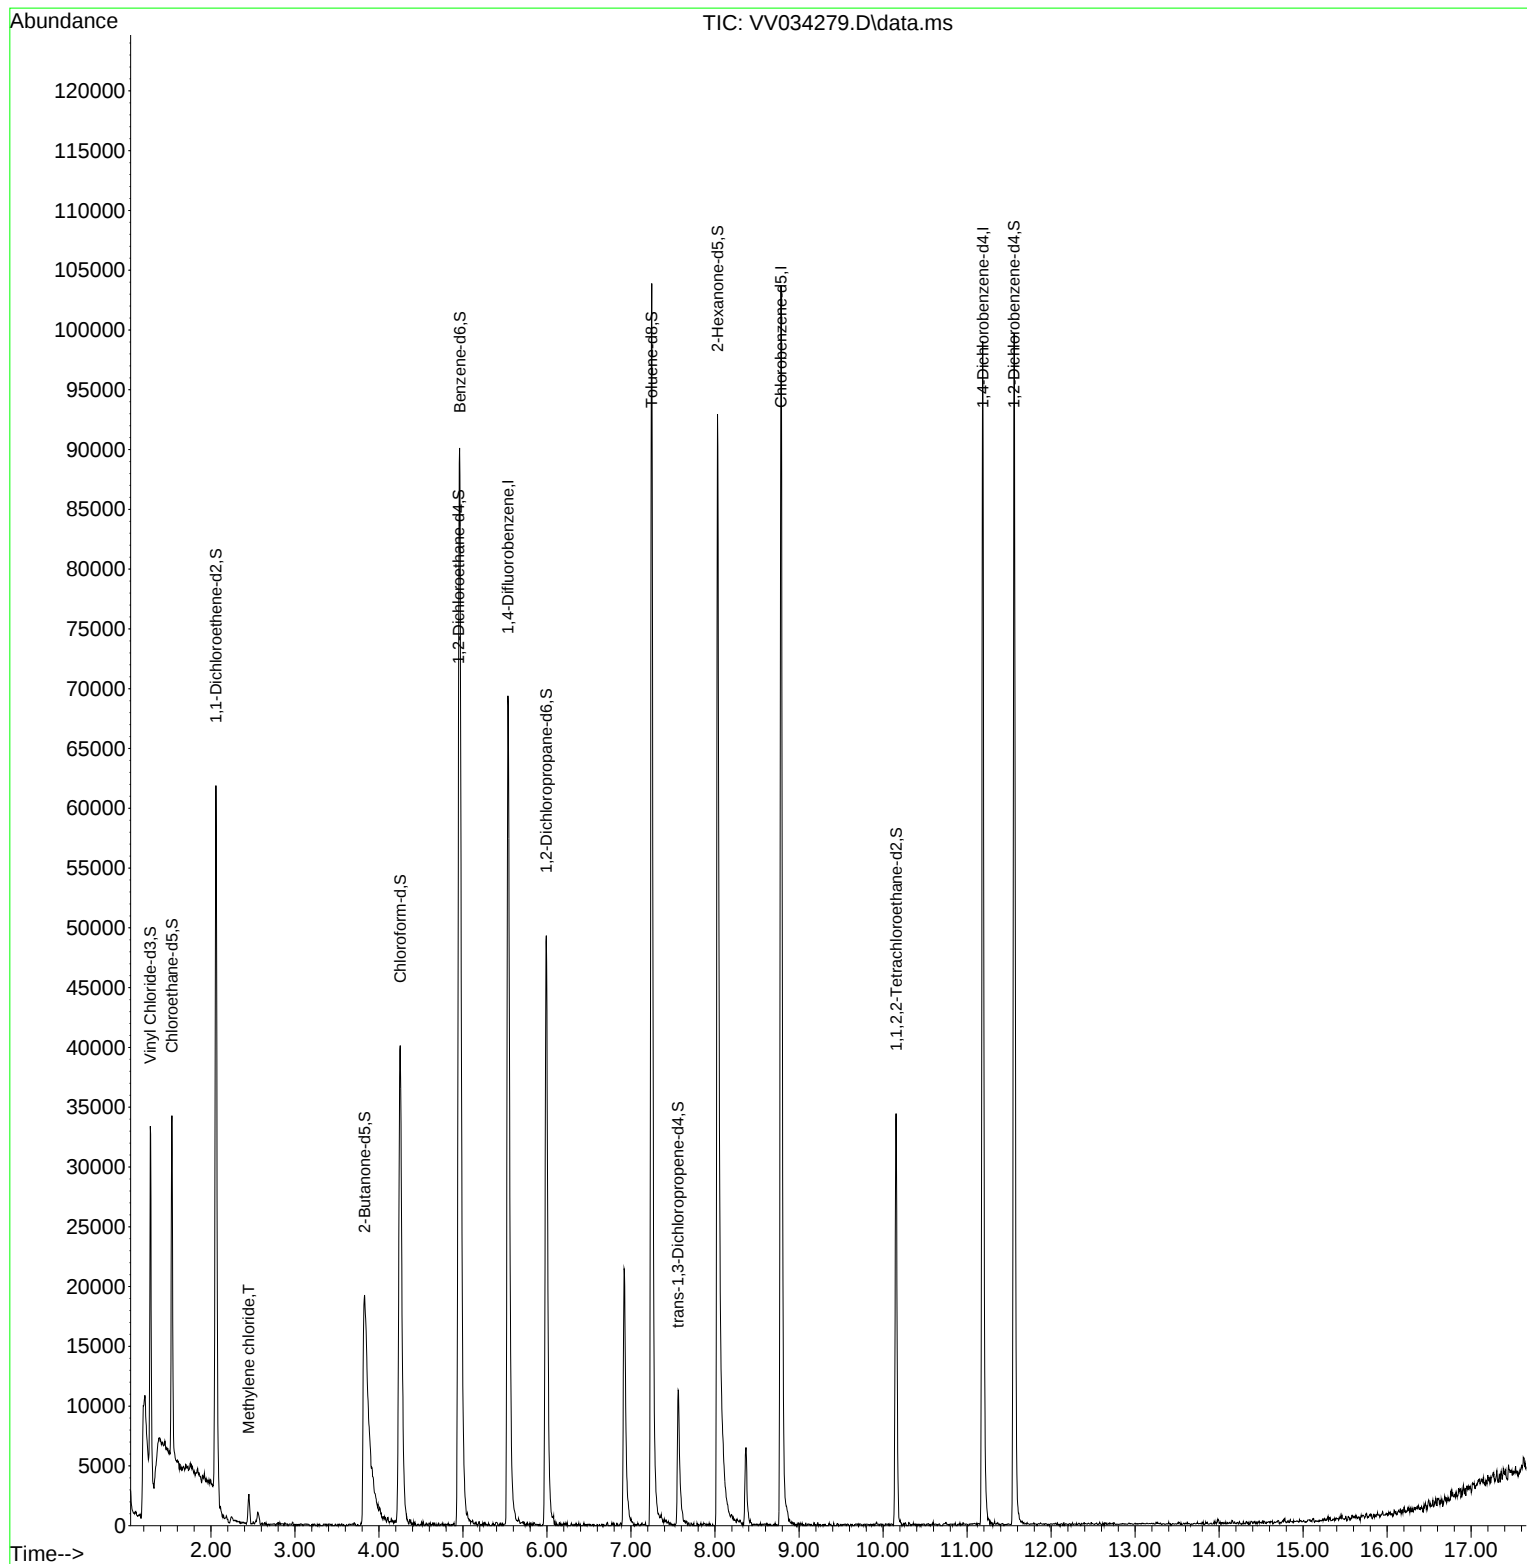

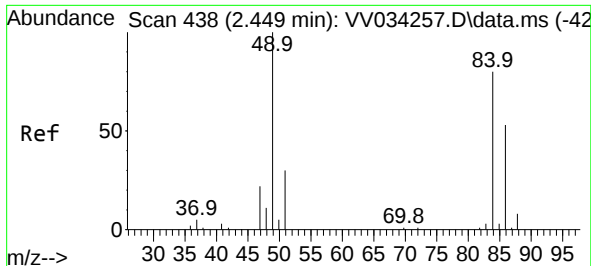

#16
Methylene chloride
Concen: 0.231 ug/L
RT: 2.449 min Scan# 41
Delta R.T. 0.000 min
Lab File: VV034279.D
Acq: 20 Feb 2024 18:58

Instrument :
MSVOA_V
ClientSampleId :
C0AB7

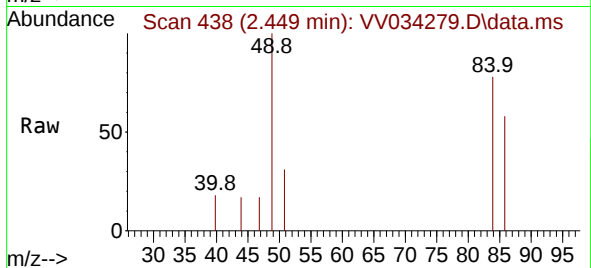

Tgt Ion: 84 Resp: 949

Ion	Ratio	Lower	Upper
84	100		
86	74.5	44.7	83.1
49	128.6	93.7	173.9

