

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW022024\
 Data File : VW034292.D
 Acq On : 21 Feb 2024 00:40
 Operator : SY/MD
 Sample : P1535-04 500X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AE7

Quant Time: Feb 21 04:50:06 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Feb 21 04:37:10 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	76659	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	68433	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	31997	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	21208	3.572	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	71.400%	
7) Chloroethane-d5	1.532	69	20224	3.889	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	77.800%	
11) 1,1-Dichloroethene-d2	2.060	65	10353	3.616	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	72.400%	
20) 2-Butanone-d5	3.838	46	27291	27.370	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	54.740%	
24) Chloroform-d	4.249	84	47457	4.399	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	88.000%	
26) 1,2-Dichloroethane-d4	4.947	65	24078	4.776	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	95.600%	
32) Benzene-d6	4.963	84	86950	4.235	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	84.600%	
36) 1,2-Dichloropropane-d6	5.989	67	25814	4.498	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	90.000%	
41) Toluene-d8	7.243	98	77828	4.124	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	82.400%	
43) trans-1,3-Dichloroprop...	7.561	79	8481	3.914	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	78.200%	
46) 2-Hexanone-d5	8.030	63	32081	41.469	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	82.940%	
56) 1,1,2,2-Tetrachloroeth...	10.156	84	16402	4.714	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	94.200%	
66) 1,2-Dichlorobenzene-d4	11.561	152	25756	4.426	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	88.600%	
Target Compounds						Qvalue
16) Methylene chloride	2.449	84	950	0.185	ug/L	78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022024\
Data File : VV034292.D
Acq On : 21 Feb 2024 00:40
Operator : SY/MD
Sample : P1535-04 500X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE7


Quant Time: Feb 21 04:50:06 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Feb 21 04:37:10 2024
Response via : Initial Calibration

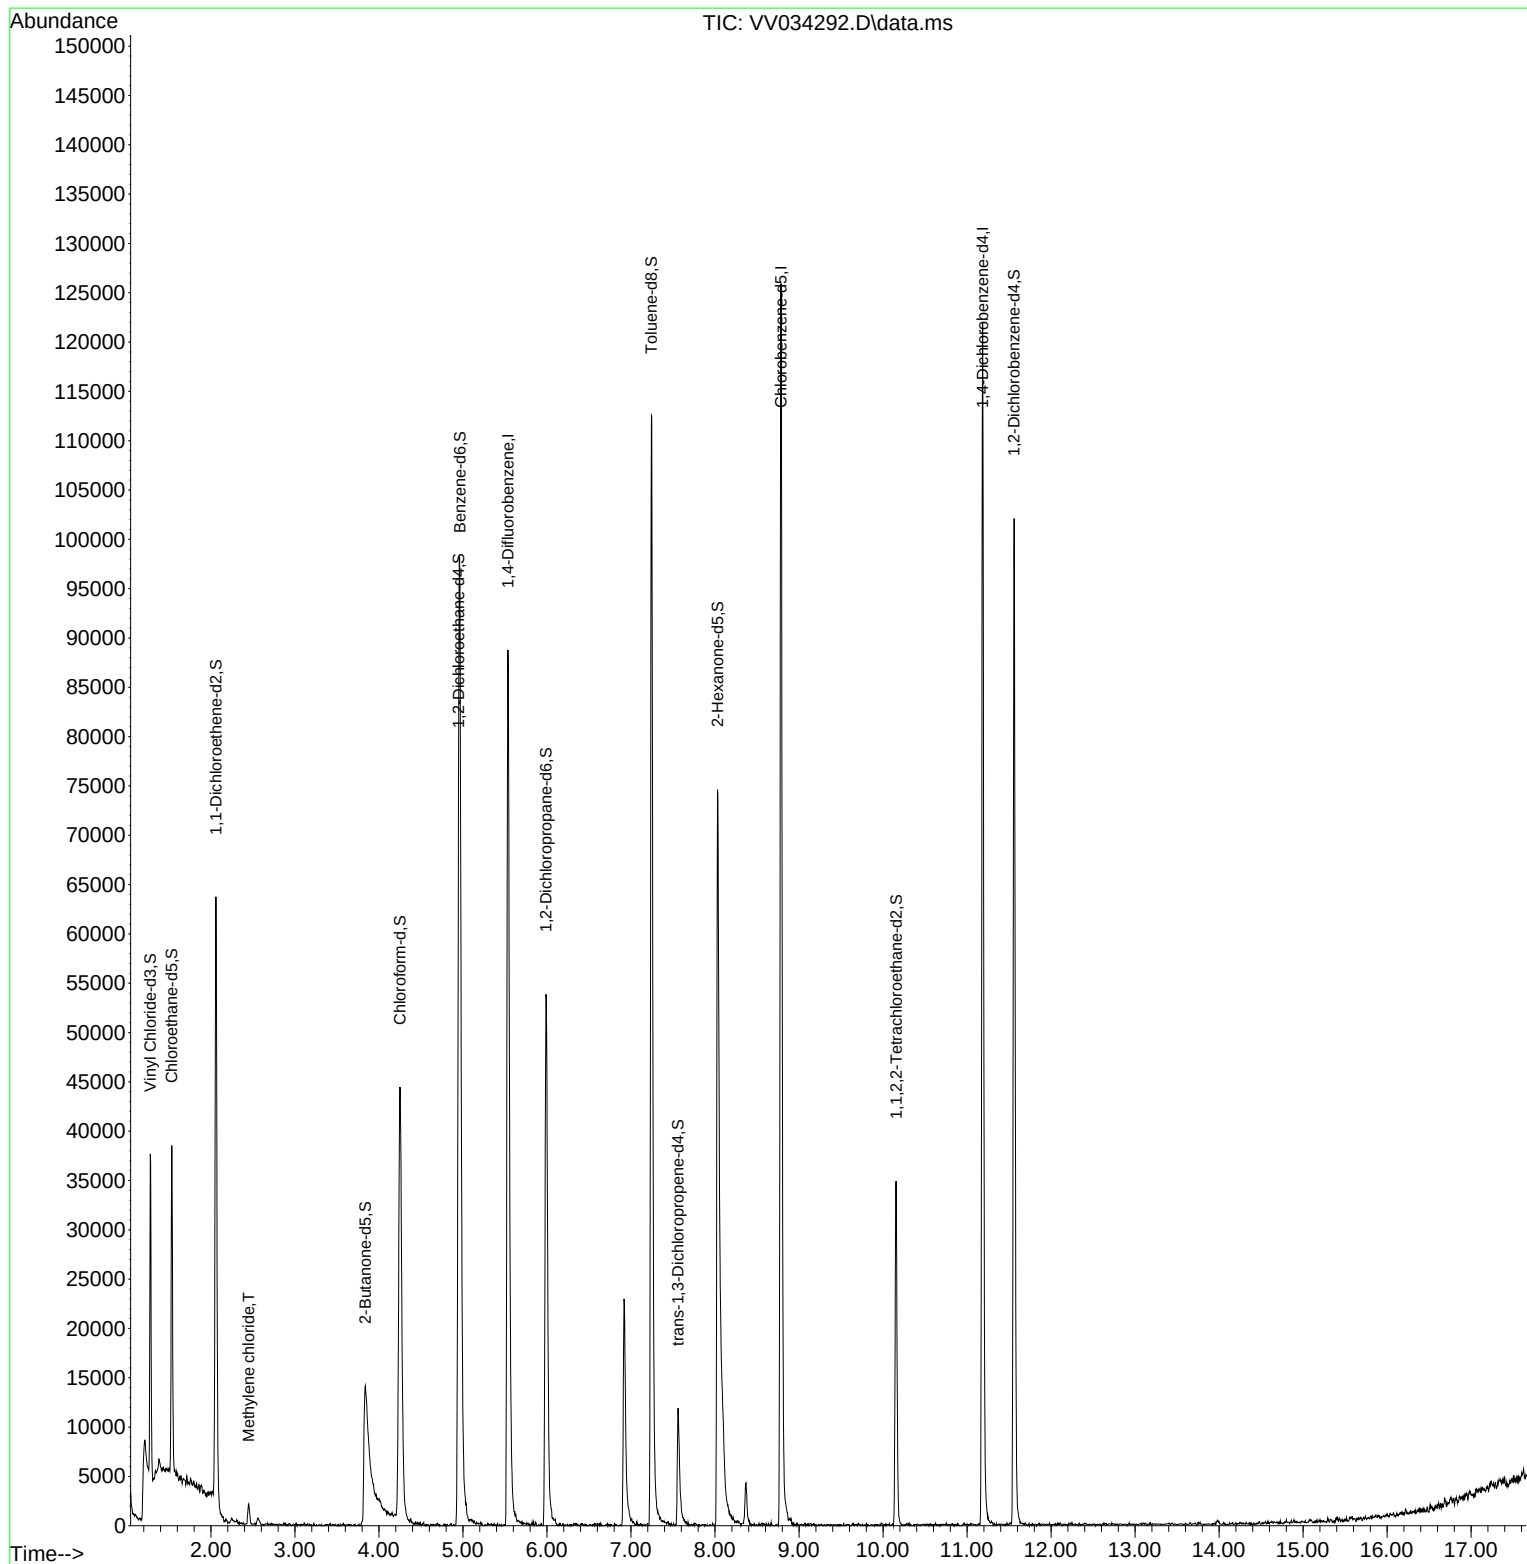

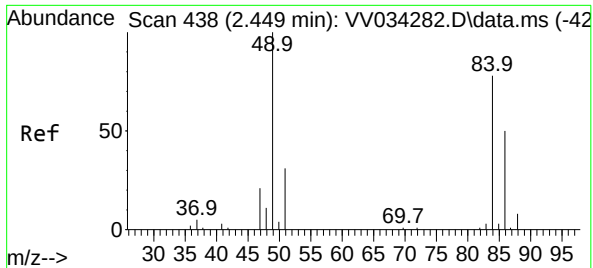

#16
Methylene chloride
Concen: 0.185 ug/L
RT: 2.449 min Scan# 41
Delta R.T. 0.000 min
Lab File: VV034292.D
Acq: 21 Feb 2024 00:40

Instrument :
MSVOA_V
ClientSampleId :
C0AE7

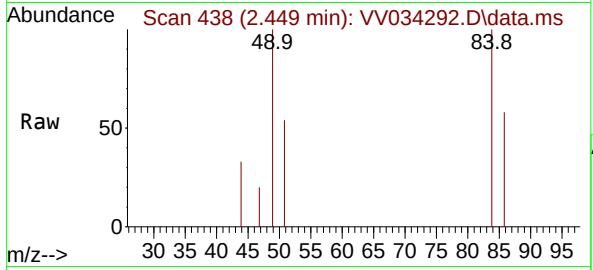

Tgt Ion:	84	Resp:	950
Ion	Ratio	Lower	Upper
84	100		
86	57.8	44.7	83.1
49	99.8	93.7	173.9

