

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022024\
 Data File : VV034279.D
 Acq On : 20 Feb 2024 18:58
 Operator : SY/MD
 Sample : P1498-17 500X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV034279.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.195	40	48	49	rBV	9400	8780	3.87%	0.475%
2	1.278	68	74	87	rVB	30272	34563	15.25%	1.869%
3	1.384	88	107	110	rBV3	4219	11960	5.28%	0.647%
4	1.536	147	154	172	rVB	28918	35218	15.54%	1.905%
5	2.060	307	317	333	rVB	60418	91874	40.54%	4.968%
6	2.452	429	439	446	rBV2	2502	3592	1.59%	0.194%
7	3.828	855	867	892	rBV3	19118	76087	33.58%	4.115%
8	4.252	984	999	1025	rBV	39885	102933	45.42%	5.566%
9	4.960	1205	1219	1245	rBV2	90141	226616	100.00%	12.255%
10	5.535	1387	1398	1430	rBV	69266	144489	63.76%	7.814%
11	5.992	1528	1540	1562	rBV2	49244	102156	45.08%	5.524%
12	6.918	1819	1828	1851	rBV	21500	43698	19.28%	2.363%
13	7.246	1920	1930	1954	rBV	103894	187911	82.92%	10.162%
14	7.561	2020	2028	2049	rBV3	11190	22050	9.73%	1.192%
15	8.030	2165	2174	2222	rBV	92963	201307	88.83%	10.886%
16	8.368	2270	2279	2292	rBV3	6545	11749	5.18%	0.635%
17	8.786	2399	2409	2438	rBV	103739	174142	76.84%	9.417%
18	10.156	2825	2835	2849	rBV2	34479	54271	23.95%	2.935%
19	11.185	3146	3155	3176	rBV	98964	156475	69.05%	8.462%
20	11.561	3261	3272	3293	rBV	99605	159311	70.30%	8.615%




Sum of corrected areas: 1849182

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022024\
Data File : VV034279.D
Acq On : 20 Feb 2024 18:58
Operator : SY/MD
Sample : P1498-17 500X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

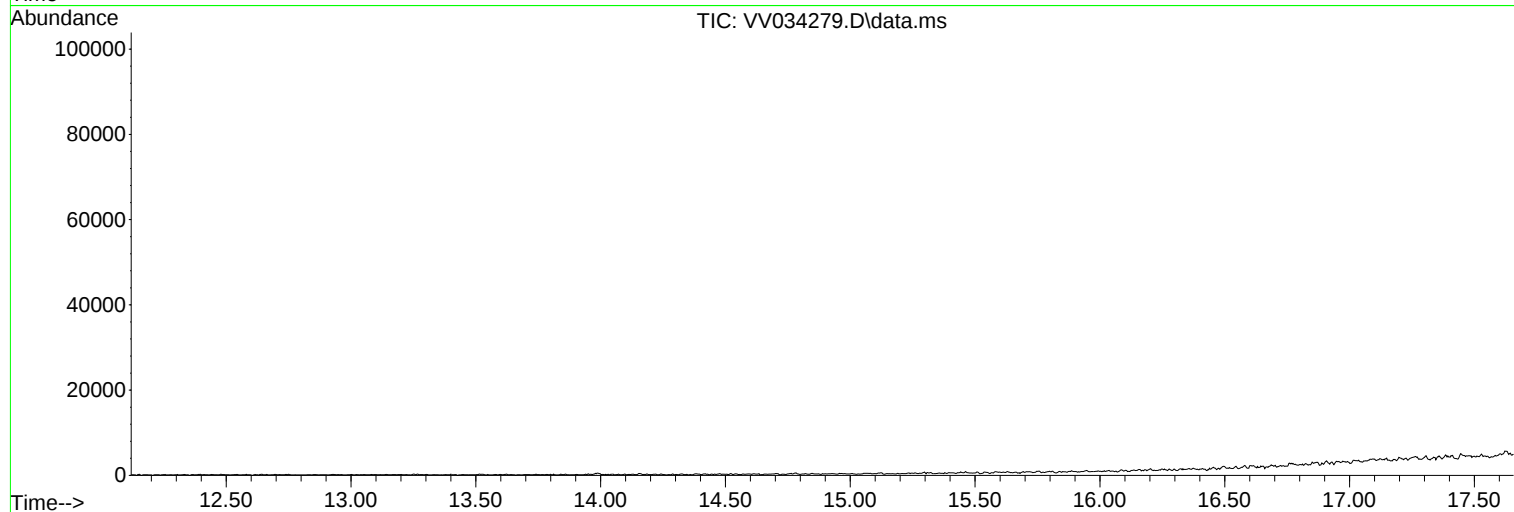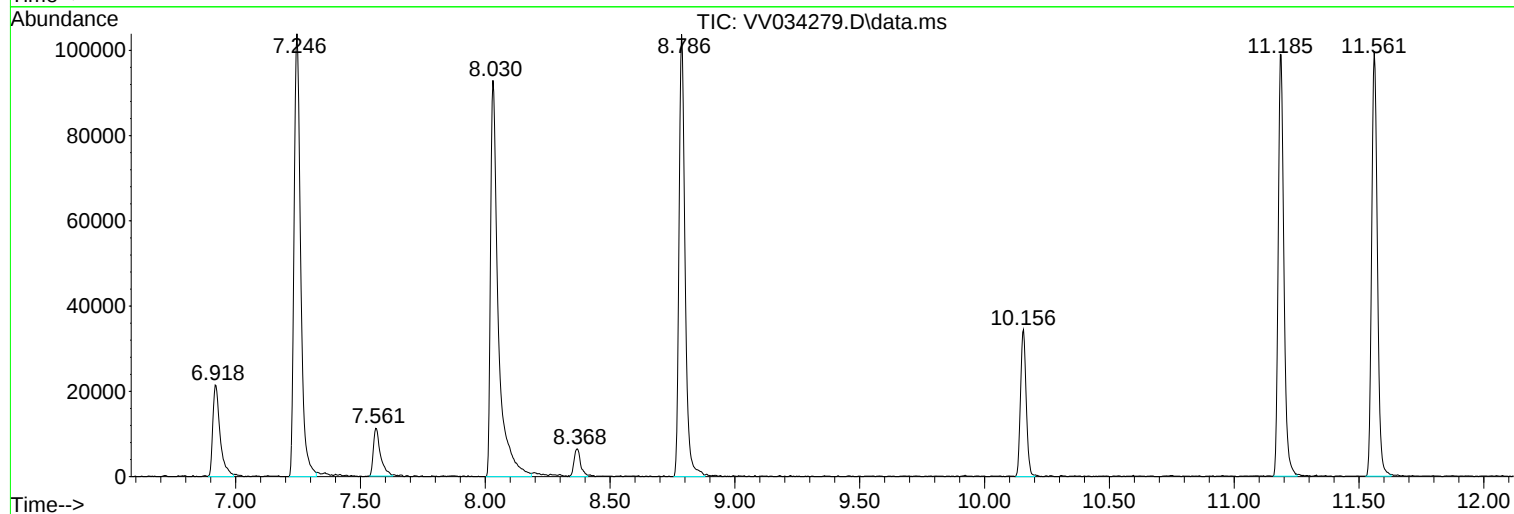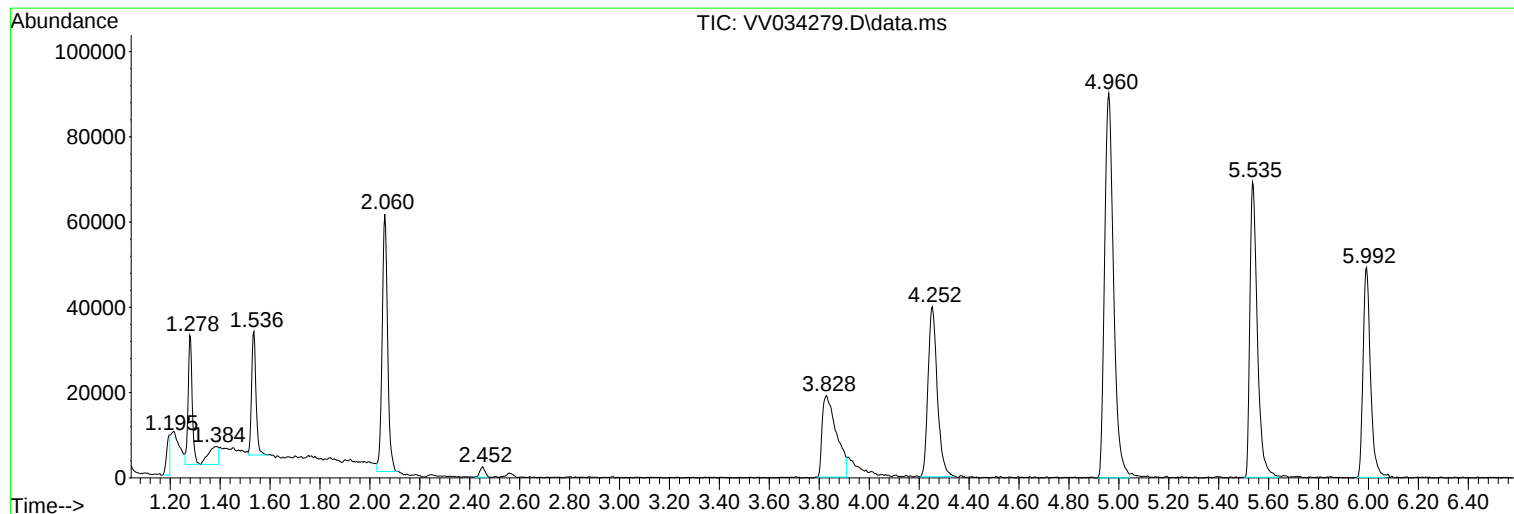

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022024\
Data File : VV034279.D
Acq On : 20 Feb 2024 18:58
Operator : SY/MD
Sample : P1498-17 500X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022024\
Data File : VV034279.D
Acq On : 20 Feb 2024 18:58
Operator : SY/MD
Sample : P1498-17 500X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc