


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022024\
Data File : VV034256.D
Acq On : 20 Feb 2024 08:31
Operator : SY/MD
Sample : BFB256
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB256

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Feb 22 00:18:57 2024

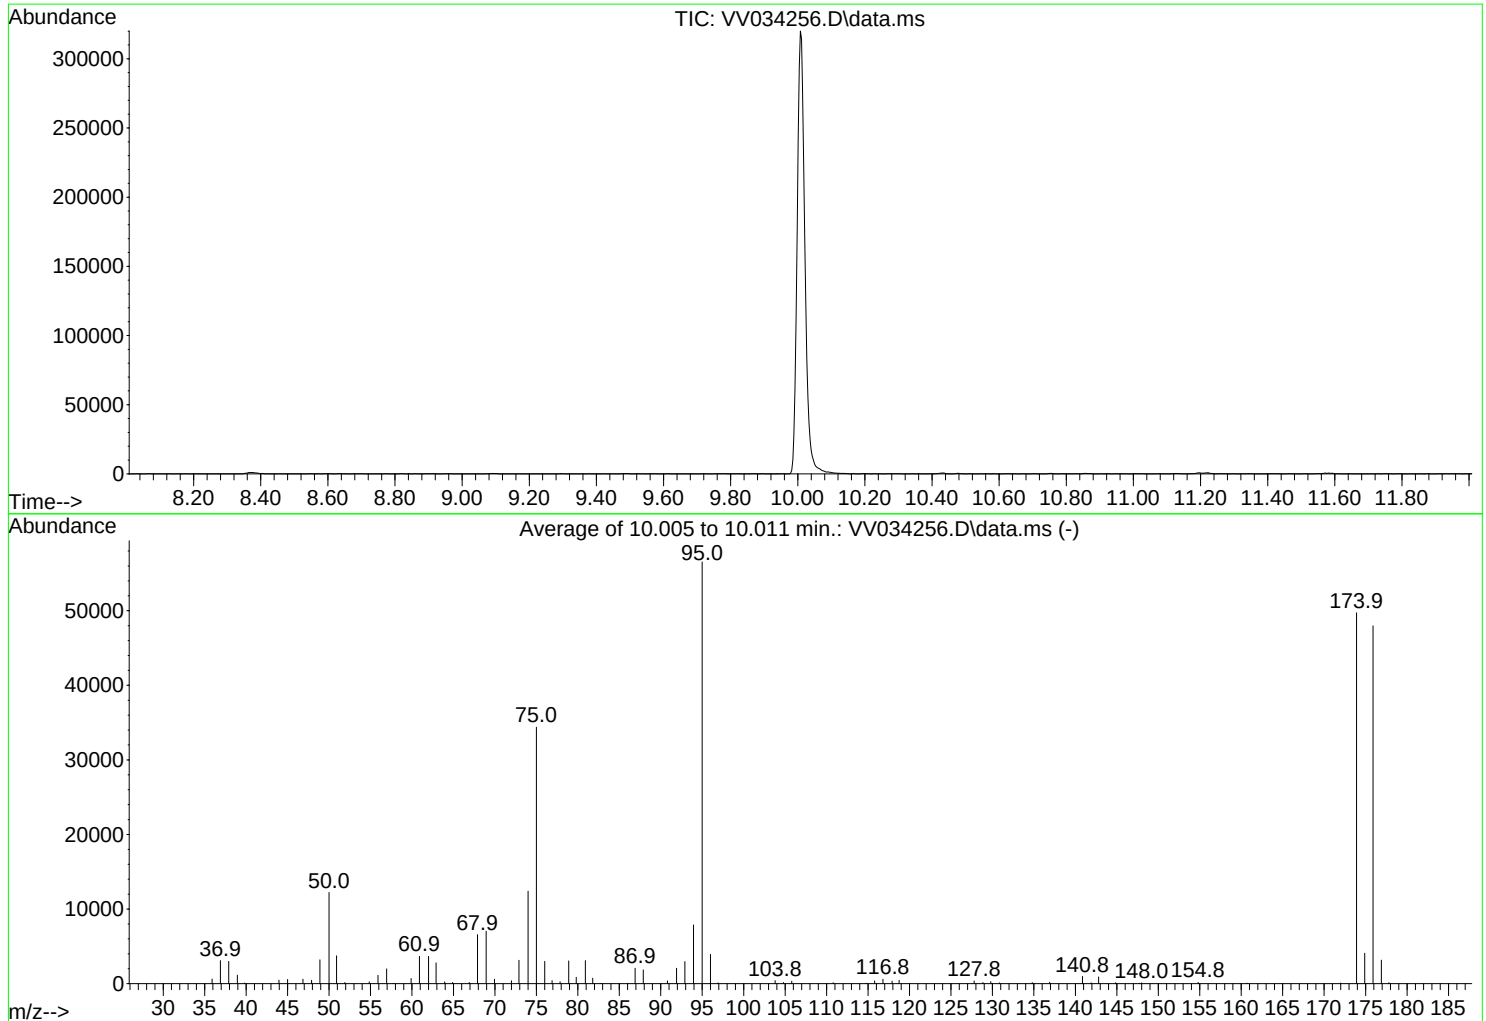

AutoFind: Scans 2788, 2789, 2790; Background Corrected with Scan 2777

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.6	12224	PASS
75	95	30	80	60.8	34400	PASS
95	95	100	100	100.0	56555	PASS
96	95	5	9	6.9	3927	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	87.9	49733	PASS
175	174	5	9	8.2	4071	PASS
176	174	95	105	96.4	47960	PASS
177	176	5	10	6.6	3146	PASS

m/z	Abundance
74.80	119.0
94.90	104.0

Instrument :
MSVOA_V
ClientSampleId :
BFB256

m/z	Abundance
35.90	627.0
36.90	3088.0
37.90	2927.0
38.90	1183.0
44.00	477.0
45.00	543.0
46.90	599.0
47.90	440.0
48.90	3147.0
50.00	11876.0
50.90	3626.0
51.90	173.0
54.90	262.0
55.90	1055.0
57.00	2019.0
57.80	118.0
59.90	643.0
60.90	3666.0
62.00	3610.0
62.90	2827.0
63.90	239.0
64.90	150.0
66.90	183.0
67.90	6519.0
68.90	6803.0
69.90	553.0
72.00	404.0
72.90	3109.0
74.00	11949.0
75.00	32760.0
76.00	3058.0
76.90	397.0
77.80	257.0
78.90	2967.0
79.80	853.0
80.90	2891.0
81.80	701.0
86.90	1843.0
87.90	1701.0
90.80	356.0
91.90	2001.0
92.90	2764.0
94.00	7713.0
95.00	53288.0
96.00	3963.0
96.90	110.0
103.80	380.0
104.80	126.0
105.80	244.0
110.80	109.0
115.80	310.0
116.80	572.0
117.90	307.0
118.70	431.0
127.80	345.0
128.90	121.0
129.80	243.0
130.90	120.0
134.80	148.0
136.90	203.0
140.80	886.0
142.80	869.0
144.90	114.0
148.00	106.0
154.80	168.0
160.70	113.0
172.00	270.0
173.90	46392.0
174.90	3929.0
175.90	43912.0
176.90	2937.0
177.80	124.0

Instrument :
MSVOA_V
ClientSampleId :
BFB256

m/z	Abundance
35.90	635.0
36.90	3185.0
37.90	3094.0
38.90	1179.0
39.80	116.0
43.90	465.0
45.00	565.0
46.80	621.0
47.90	484.0
48.90	3327.0
50.00	12684.0
50.90	3851.0
51.90	161.0
54.90	251.0
55.90	1139.0
57.00	2074.0
59.90	717.0
60.90	3760.0
62.00	3792.0
62.90	2882.0
63.90	217.0
64.90	169.0
66.90	185.0
67.90	6824.0
69.00	7262.0
69.90	600.0
72.00	416.0
72.90	3186.0
74.00	12798.0
75.00	35696.0
76.00	3058.0
76.90	423.0
77.80	261.0
78.90	3168.0
79.80	876.0
80.90	3216.0
81.80	757.0
86.90	2134.0
87.90	1904.0
90.80	392.0
91.90	2128.0
92.90	3018.0
94.00	8169.0
95.00	58624.0
96.00	4030.0
96.90	114.0
103.80	422.0
104.80	150.0
105.80	317.0
110.80	146.0
114.70	106.0
115.80	373.0
116.80	641.0
117.90	350.0
118.70	475.0
127.80	379.0
128.80	159.0
129.80	286.0
130.90	120.0
134.80	163.0
136.90	190.0
140.80	992.0
141.90	127.0
142.80	917.0
144.90	132.0
148.00	105.0
154.80	181.0
160.70	105.0
173.90	51504.0
174.90	4181.0
175.90	49584.0
176.90	3231.0
177.80	140.0

Instrument :
MSVOA_V
ClientSampleId :
BFB256

m/z	Abundance
35.90	598.0
36.90	3011.0
37.90	2934.0
39.00	1029.0
39.80	119.0
43.90	452.0
45.00	544.0
46.80	582.0
47.90	442.0
48.90	3108.0
50.00	12113.0
50.90	3729.0
51.90	135.0
54.80	192.0
55.90	1176.0
56.90	1838.0
59.90	731.0
60.90	3555.0
62.00	3551.0
62.90	2695.0
64.00	224.0
64.90	160.0
66.90	160.0
67.90	6370.0
69.00	7029.0
70.00	653.0
72.00	370.0
72.90	3088.0
74.00	12478.0
75.00	34744.0
76.00	2821.0
76.90	411.0
77.90	275.0
78.90	2993.0
79.80	826.0
80.90	3189.0
81.80	719.0
82.80	102.0
86.00	106.0
86.90	2200.0
87.90	1946.0
90.80	380.0
91.90	2061.0
92.90	3082.0
93.90	7726.0
95.00	57752.0
96.00	3788.0
96.90	108.0
103.80	394.0
104.80	173.0
105.80	378.0
110.80	153.0
114.80	105.0
115.80	390.0
116.80	617.0
117.90	348.0
118.80	470.0
127.80	347.0
128.80	185.0
129.80	310.0
130.80	116.0
134.80	162.0
136.90	166.0
140.90	994.0
141.90	169.0
142.80	896.0
144.80	136.0
147.70	101.0
148.00	106.0
154.80	187.0
173.90	51304.0
174.90	4102.0
175.90	50384.0
176.90	3271.0
177.80	123.0

Instrument :
MSVOA_V
ClientSampleId :
BFB256