

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW022122\
 Data File : VW024786.D
 Acq On : 21 Feb 2022 19:25
 Operator : SY/MD
 Sample : N1623-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBD41

Quant Time: Feb 22 03:32:08 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Feb 22 03:27:30 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	163454	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	150739	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	65807	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	47073	3.395	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	68.000%
7) Chloroethane-d5	1.568	69	42892	3.771	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	75.400%
11) 1,1-Dichloroethene-d2	2.111	63	63922	2.516	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	50.400%#
20) 2-Butanone-d5	3.886	46	99489	50.239	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	100.480%
24) Chloroform-d	4.352	84	89483	4.136	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	82.800%
26) 1,2-Dichloroethane-d4	5.034	65	41505	4.304	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.000%
32) Benzene-d6	5.050	84	179905	4.137	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	82.800%
36) 1,2-Dichloropropane-d6	6.069	67	57011	4.455	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	89.000%
41) Toluene-d8	7.317	98	152311	3.855	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	77.000%
43) trans-1,3-Dichloroprop...	7.625	79	17174	4.028	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	80.600%
46) 2-Hexanone-d5	8.088	63	75814	45.194	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	90.380%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	33789	4.381	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	87.600%
66) 1,2-Dichlorobenzene-d4	11.622	152	51495	4.522	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	90.400%
Target Compounds					Qvalue	
25) Chloroform	4.375	83	1781	0.075	ug/L	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022122\
Data File : VV024786.D
Acq On : 21 Feb 2022 19:25
Operator : SY/MD
Sample : N1623-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBD41

Quant Time: Feb 22 03:32:08 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Feb 22 03:27:30 2022
Response via : Initial Calibration

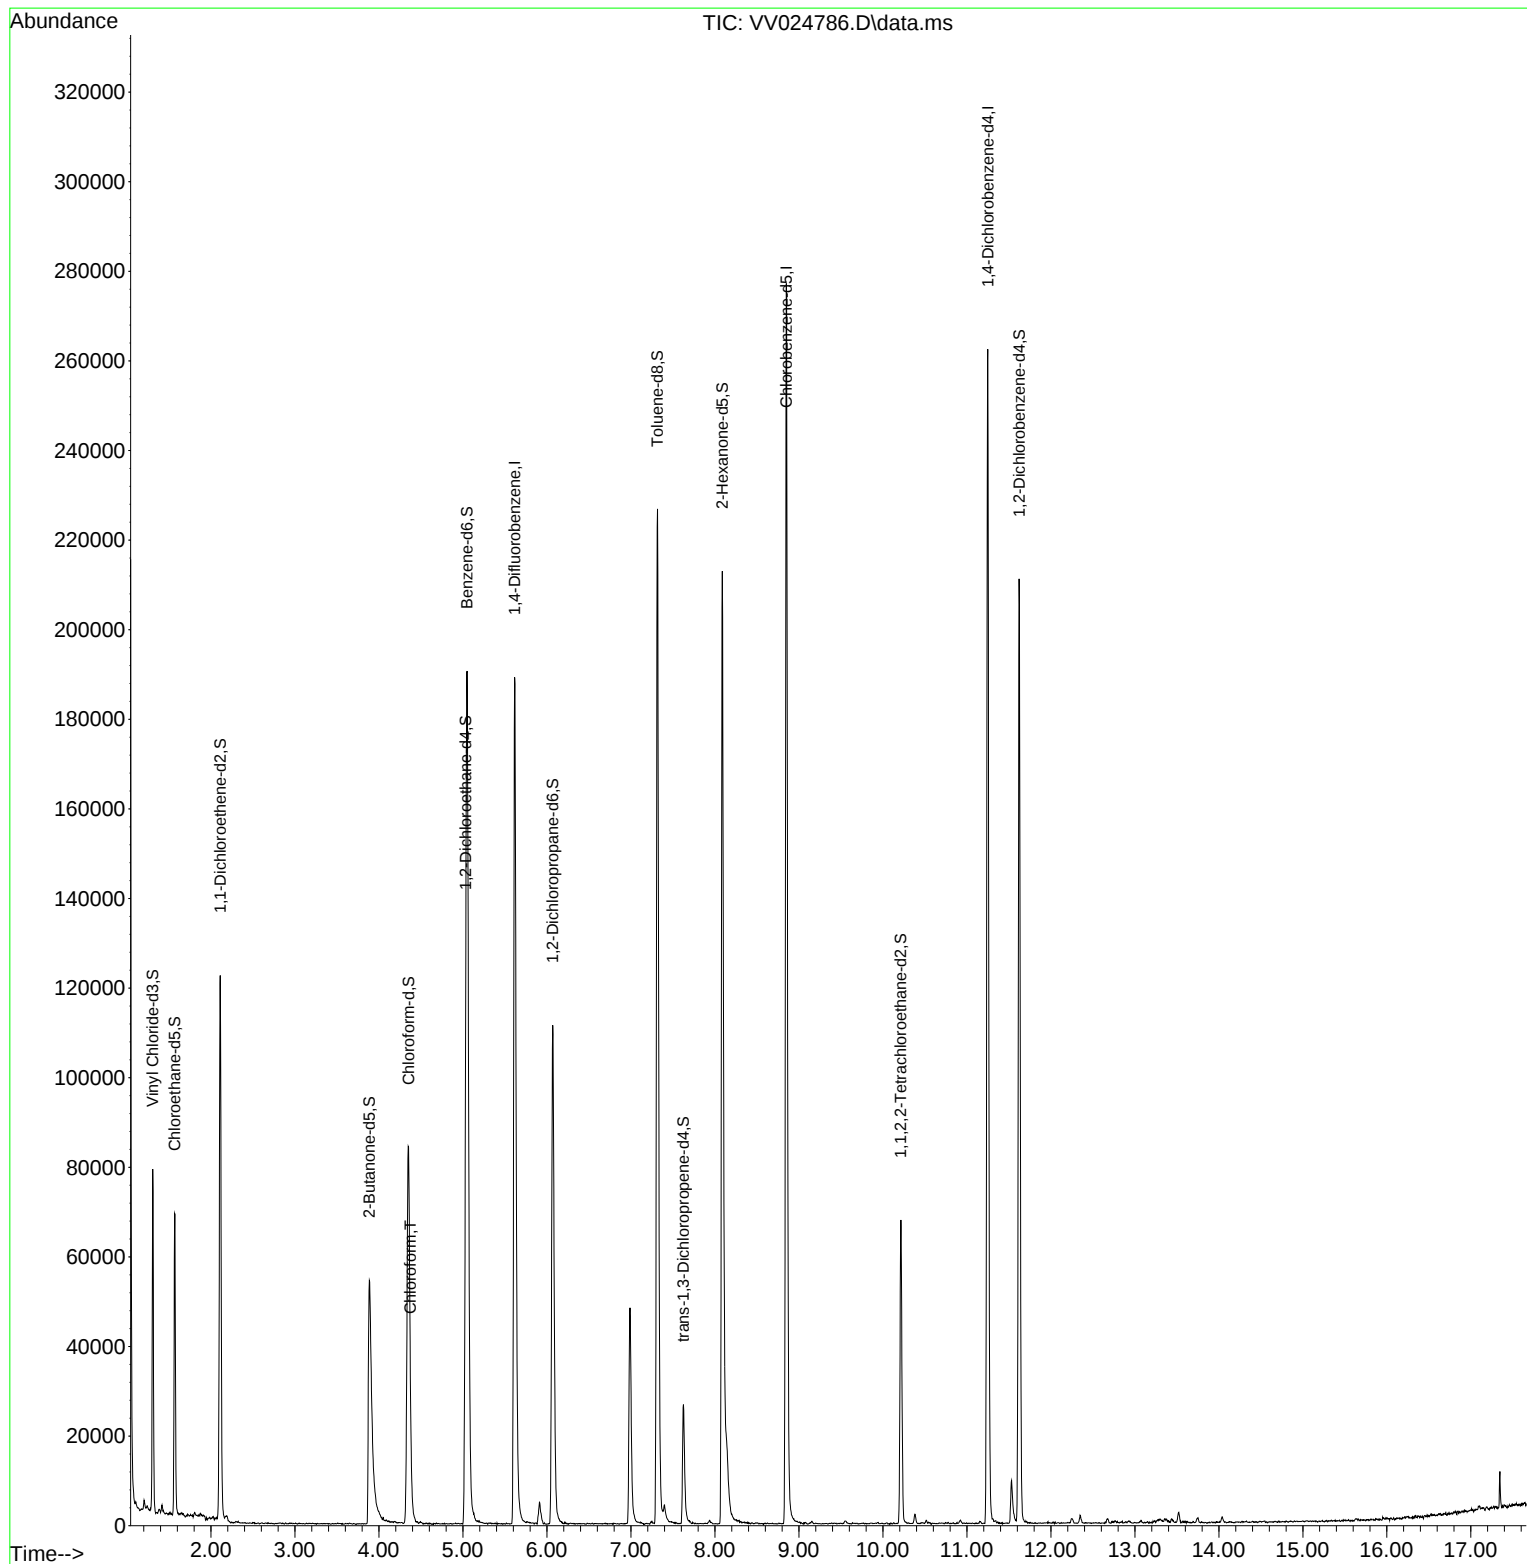

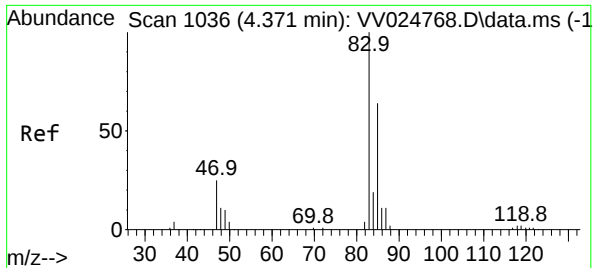

#25
Chloroform
Concen: 0.075 ug/L
RT: 4.375 min Scan# 10
Delta R.T. 0.003 min
Lab File: VV024786.D
Acq: 21 Feb 2022 19:25

Instrument :
MSVOA_V
ClientSampleId :
GBD41

Tgt Ion: 83 Resp: 1781
Ion Ratio Lower Upper
83 100
85 76.4 45.5 84.5

