

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW022122\
 Data File : VW024787.D
 Acq On : 21 Feb 2022 19:49
 Operator : SY/MD
 Sample : N1623-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBD42

Quant Time: Feb 22 03:32:22 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Feb 22 03:27:30 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	162791	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	149838	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	65638	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	46630	3.377	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	67.600%	
7) Chloroethane-d5	1.568	69	42549	3.756	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	75.200%	
11) 1,1-Dichloroethene-d2	2.111	63	63739	2.519	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	50.400%#	
20) 2-Butanone-d5	3.889	46	98417	49.900	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	99.800%	
24) Chloroform-d	4.352	84	89859	4.171	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	83.400%	
26) 1,2-Dichloroethane-d4	5.034	65	41897	4.363	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	87.200%	
32) Benzene-d6	5.050	84	180045	4.165	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	83.400%	
36) 1,2-Dichloropropane-d6	6.072	67	56915	4.474	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	89.400%	
41) Toluene-d8	7.317	98	153151	3.899	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	78.000%	
43) trans-1,3-Dichloroprop...	7.625	79	17356	4.096	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	82.000%	
46) 2-Hexanone-d5	8.088	63	75357	45.191	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	90.380%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	33719	4.398	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	88.000%	
66) 1,2-Dichlorobenzene-d4	11.622	152	50008	4.403	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	88.000%	
Target Compounds						
25) Chloroform	4.381	83	1784	0.075	ug/L	Qvalue 85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022122\
Data File : VV024787.D
Acq On : 21 Feb 2022 19:49
Operator : SY/MD
Sample : N1623-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBD42

Quant Time: Feb 22 03:32:22 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Feb 22 03:27:30 2022
Response via : Initial Calibration

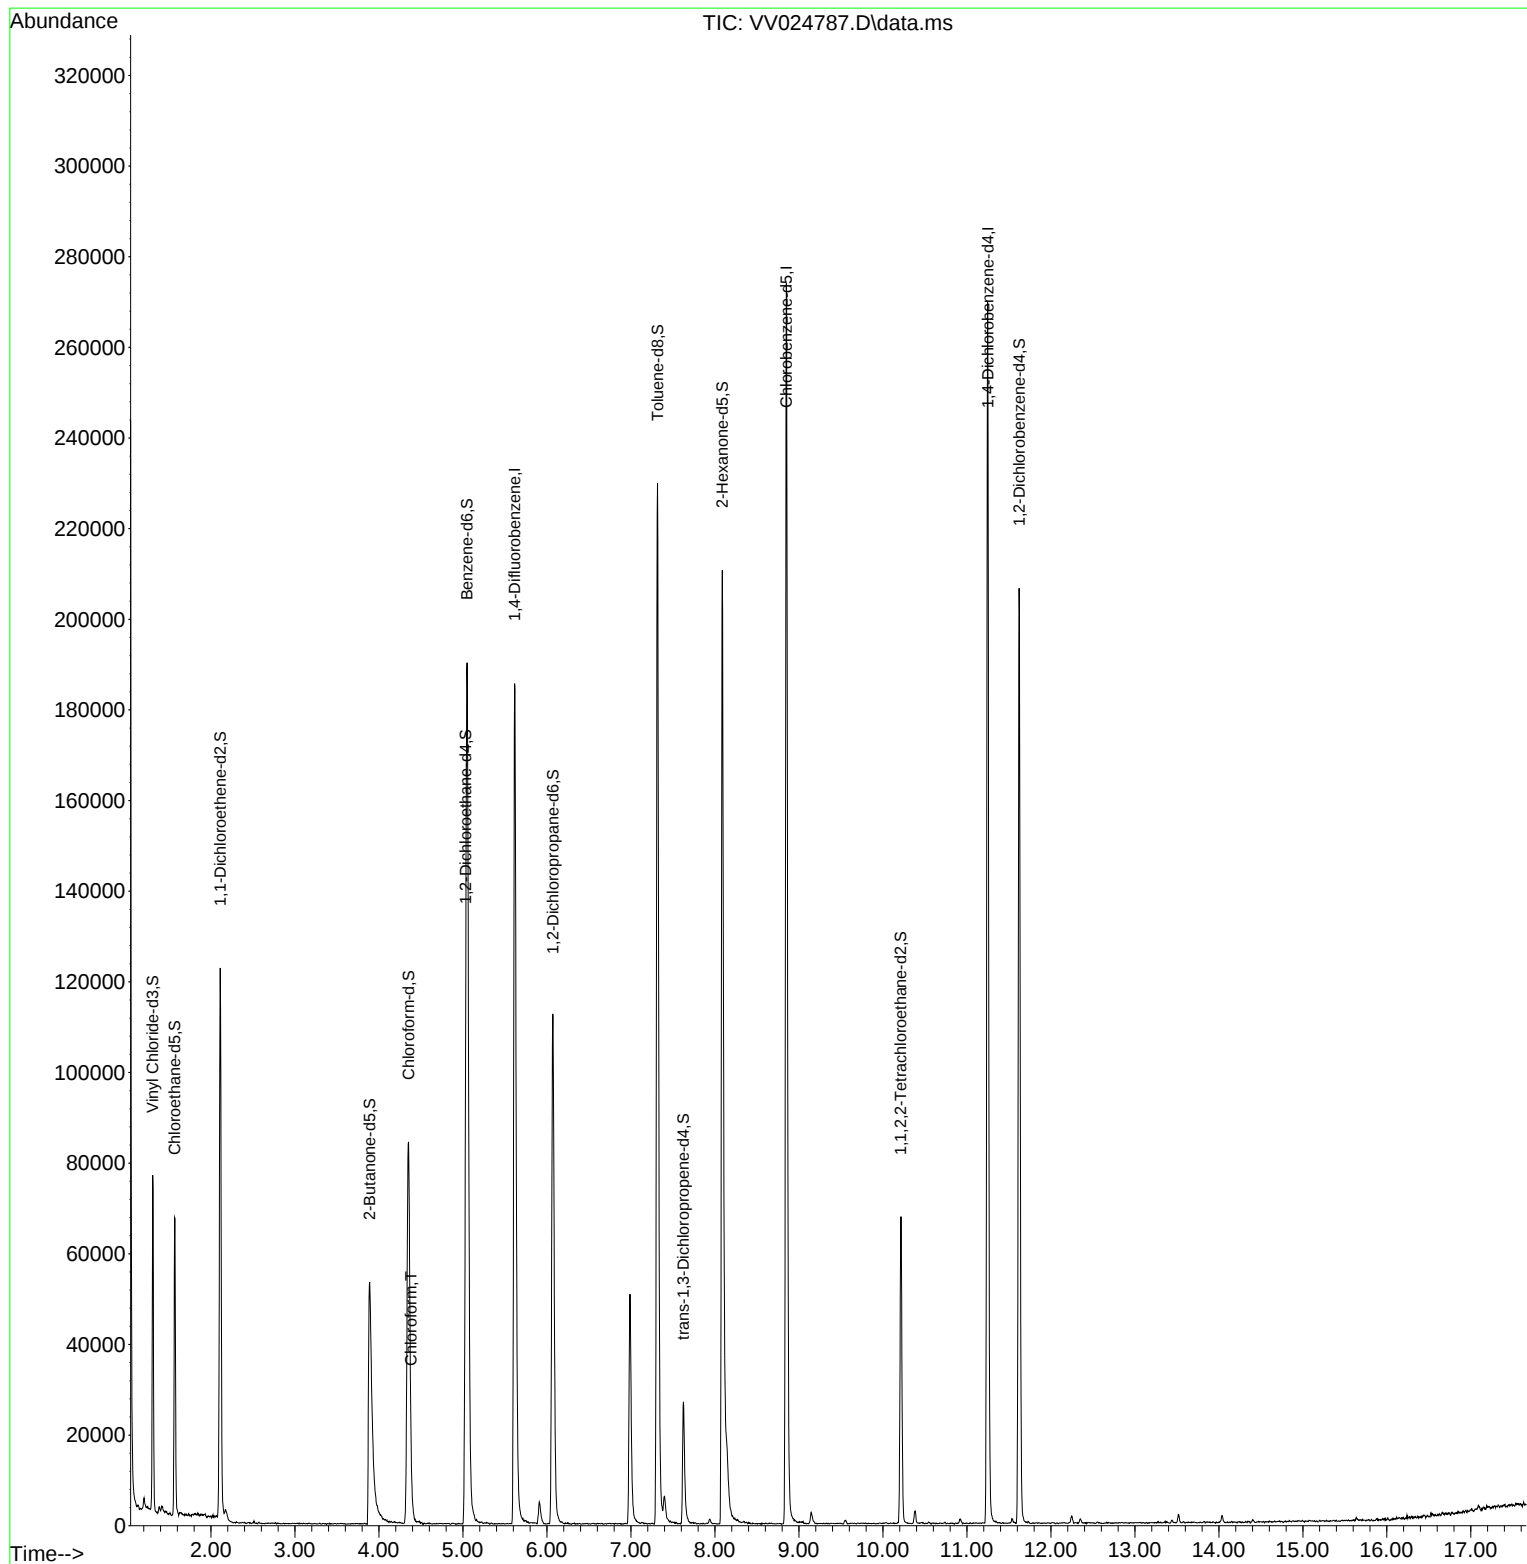

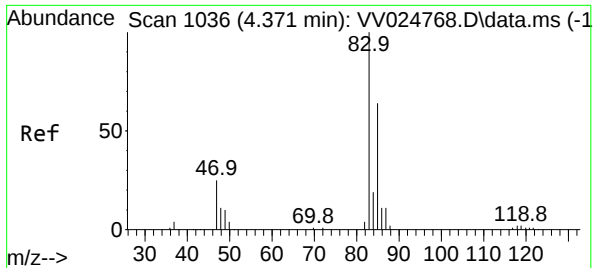

#25
 Chloroform
 Concen: 0.075 ug/L
 RT: 4.381 min Scan# 10
 Delta R.T. 0.010 min
 Lab File: VV024787.D
 Acq: 21 Feb 2022 19:49

Instrument :
 MSVOA_V
 ClientSampleId :
 GBD42

Tgt Ion: 83 Resp: 1784
 Ion Ratio Lower Upper
 83 100
 85 76.5 45.5 84.5

