

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022122\
 Data File : VV024772.D
 Acq On : 21 Feb 2022 13:39
 Operator : SY/MD
 Sample : VIBLK259
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK259

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV024772.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	95	rVB	83194	84790	16.82%	1.972%
2	1.568	156	164	175	rBV	74547	82954	16.46%	1.929%
3	2.108	321	332	352	rBV	132953	195790	38.84%	4.553%
4	2.507	445	456	472	rBV	25722	43232	8.58%	1.005%
5	3.886	876	885	923	rBV2	50530	157939	31.33%	3.673%
6	4.346	1010	1028	1059	rBV	88425	225385	44.72%	5.241%
7	5.047	1230	1246	1276	rBV2	204039	504036	100.00%	11.721%
8	5.613	1411	1422	1449	rBV	192556	391089	77.59%	9.095%
9	5.908	1504	1514	1532	rVB7	5507	12302	2.44%	0.286%
10	6.066	1550	1563	1592	rBV	115625	240112	47.64%	5.584%
11	6.985	1839	1849	1872	rBV	54449	100514	19.94%	2.337%
12	7.313	1940	1951	1972	rBV	245531	431439	85.60%	10.033%
13	7.622	2036	2047	2065	rBV2	28665	51311	10.18%	1.193%
14	7.937	2135	2145	2156	rVB3	3385	5776	1.15%	0.134%
15	8.085	2181	2191	2233	rBV	210489	417969	82.92%	9.720%
16	8.850	2417	2429	2457	rBV	285576	463356	91.93%	10.775%
17	10.214	2843	2853	2869	rBV	66986	103684	20.57%	2.411%
18	10.381	2893	2905	2915	rVB2	6387	9760	1.94%	0.227%
19	11.246	3164	3174	3197	rBV	278057	428795	85.07%	9.971%
20	11.622	3280	3291	3309	rBV	223120	340822	67.62%	7.926%
21	12.249	3475	3486	3496	rVB2	6037	9199	1.83%	0.214%




Sum of corrected areas: 4300254

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022122\
Data File : VV024772.D
Acq On : 21 Feb 2022 13:39
Operator : SY/MD
Sample : VIBLK259
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK259

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

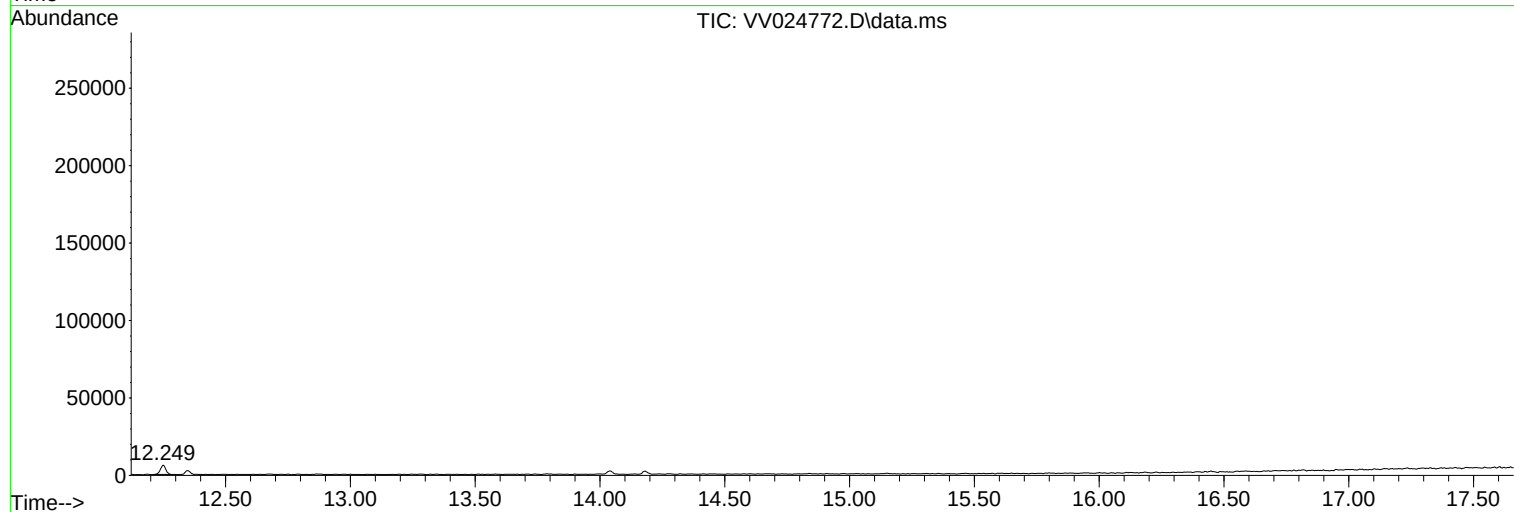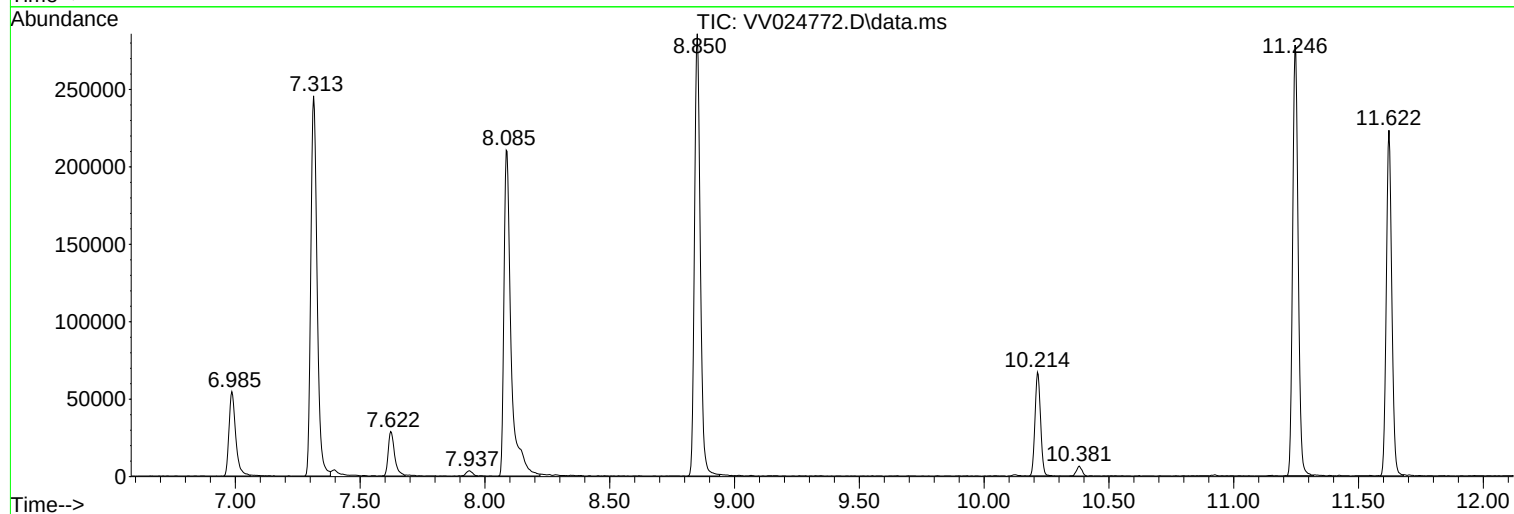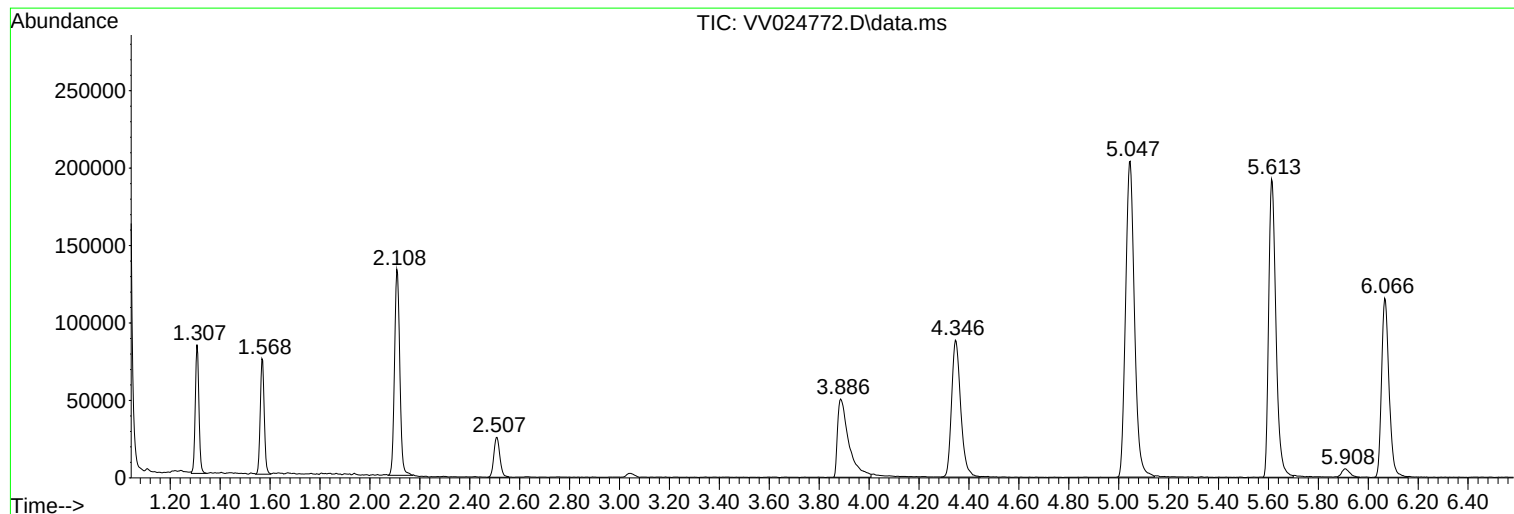

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022122\
Data File : VV024772.D
Acq On : 21 Feb 2022 13:39
Operator : SY/MD
Sample : VIBLK259
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK259

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022122\
Data File : VV024772.D
Acq On : 21 Feb 2022 13:39
Operator : SY/MD
Sample : VIBLK259
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK259

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc