

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022122\
 Data File : VV024773.D
 Acq On : 21 Feb 2022 14:02
 Operator : SY/MD
 Sample : N1623-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBD27

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV024773.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.130	19	28	40	rVB	122673	113737	11.79%	0.921%
2	1.310	76	84	99	rVB2	187313	200758	20.80%	1.626%
3	1.587	156	170	184	rBV2	255086	364074	37.72%	2.949%
4	2.117	322	335	346	rBV3	555693	965094	100.00%	7.818%
5	2.179	346	354	386	rVB	162862	369397	38.28%	2.992%
6	2.436	423	434	449	rBV	31424	57666	5.98%	0.467%
7	2.510	450	457	468	rVB3	5995	10185	1.06%	0.083%
8	2.764	525	536	559	rBV	95097	167655	17.37%	1.358%
9	3.191	656	669	686	rBV2	48058	100699	10.43%	0.816%
10	3.908	876	892	919	rBV2	125933	396327	41.07%	3.210%
11	4.252	982	999	1016	rBV2	74240	182747	18.94%	1.480%
12	4.371	1016	1036	1069	rVB3	217443	687216	71.21%	5.567%
13	4.609	1094	1110	1133	rBV3	50549	128715	13.34%	1.043%
14	4.831	1163	1179	1203	rBV	70105	170758	17.69%	1.383%
15	5.050	1231	1247	1265	rBV2	211783	520890	53.97%	4.219%
16	5.137	1265	1274	1296	rVB2	26995	62225	6.45%	0.504%
17	5.616	1412	1423	1448	rBV	198462	401962	41.65%	3.256%
18	5.915	1504	1516	1545	rVB3	87109	181456	18.80%	1.470%
19	6.069	1552	1564	1589	rBV	121050	245513	25.44%	1.989%
20	6.989	1840	1850	1855	rBV2	62613	101563	10.52%	0.823%
21	7.027	1855	1862	1888	rVB	134683	247235	25.62%	2.003%
22	7.223	1906	1923	1941	rBV	525097	924059	95.75%	7.485%
23	7.313	1941	1951	1971	rVB	259073	459117	47.57%	3.719%
24	7.625	2038	2048	2051	rBV2	37593	54017	5.60%	0.438%
25	7.651	2052	2056	2074	rVB	52028	87479	9.06%	0.709%
26	7.841	2104	2115	2134	rBV2	50538	88629	9.18%	0.718%
27	7.976	2146	2157	2181	rVB	139684	236109	24.46%	1.913%
28	8.088	2181	2192	2233	rBV	232990	450001	46.63%	3.645%
29	8.352	2263	2274	2289	rBV	54756	93180	9.66%	0.755%
30	8.850	2416	2429	2433	rBV	314727	461616	47.83%	3.739%
31	8.879	2434	2438	2464	rVB	395533	594109	61.56%	4.813%
32	9.731	2693	2703	2715	rBV2	23998	38187	3.96%	0.309%
33	10.217	2842	2854	2882	rVB2	72440	154506	16.01%	1.252%
34	10.911	3059	3070	3092	rBV	416221	625917	64.86%	5.070%
35	11.178	3143	3153	3165	rBV	195598	303111	31.41%	2.455%
36	11.249	3165	3175	3197	rVB2	312693	664238	68.83%	5.381%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022122\
Data File : VV024773.D
Acq On : 21 Feb 2022 14:02
Operator : SY/MD
Sample : N1623-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBD27

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.1 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Title : TRACE VOA SFAM1.0

37	11.622	3280	3291	3315	rBV	231323	359229	37.22%	2.910%
38	12.644	3597	3609	3625	rBV	316745	486251	50.38%	3.939%
39	13.258	3790	3800	3820	rBV	259949	389877	40.40%	3.158%
40	13.741	3939	3950	3967	rBV	129176	199365	20.66%	1.615%




Sum of corrected areas: 12344869

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022122\
Data File : VV024773.D
Acq On : 21 Feb 2022 14:02
Operator : SY/MD
Sample : N1623-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBD27

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

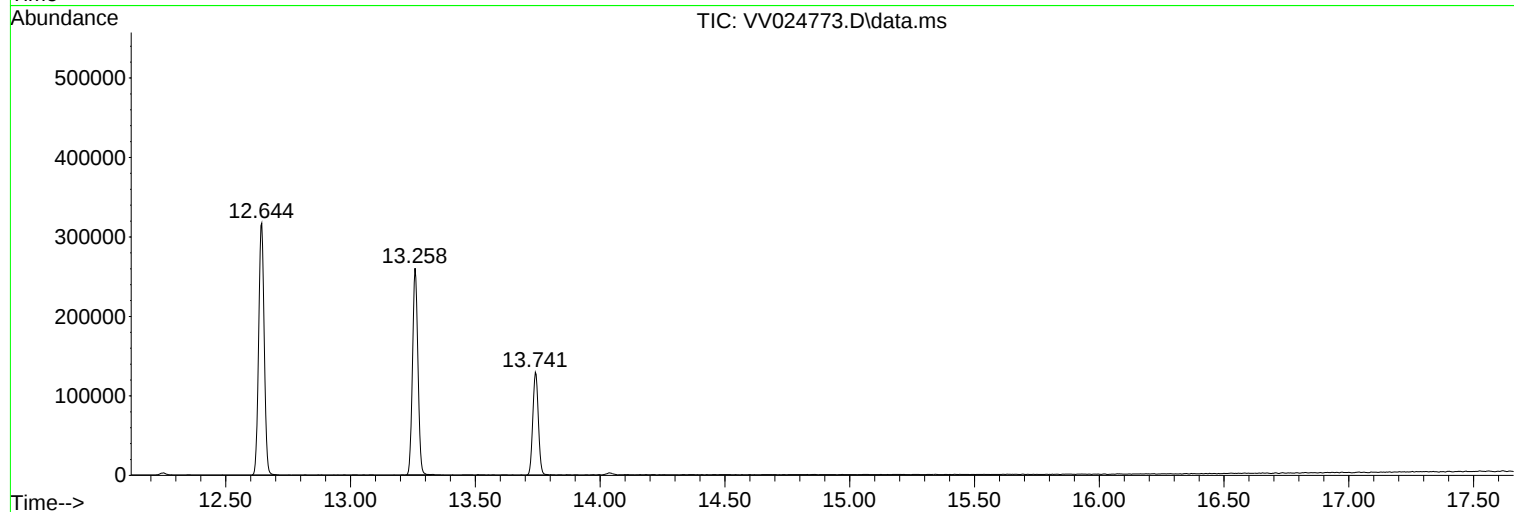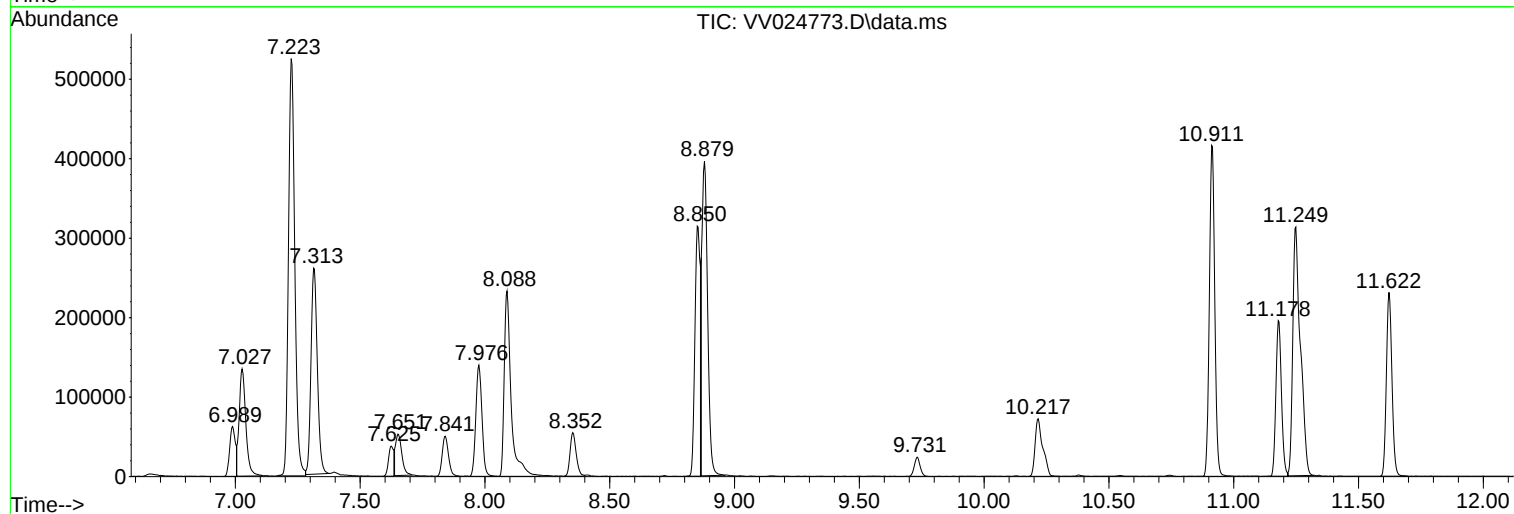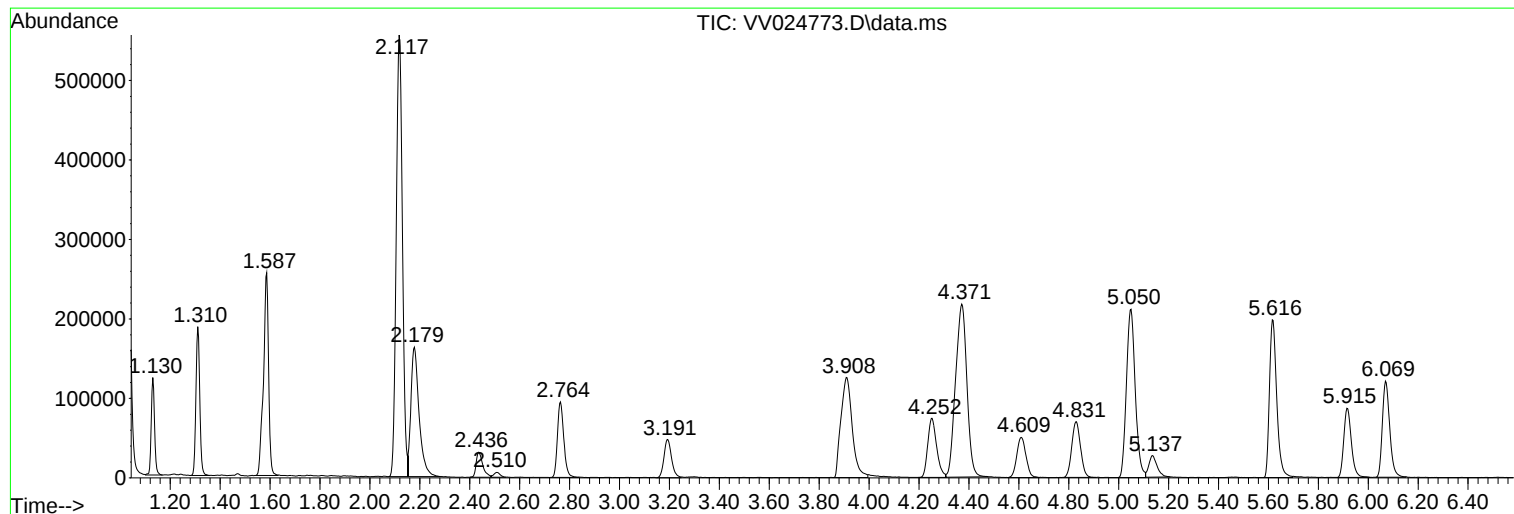

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022122\
Data File : VV024773.D
Acq On : 21 Feb 2022 14:02
Operator : SY/MD
Sample : N1623-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBD27










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzene, 1,3,5-trichloro- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
12.644	3.66 ug/L	486251	1,4-Dichlorobenzene-d4	11.246

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzene, 1,3,5-trichloro-	180	C6H3Cl3	000108-70-3	98
2			Benzene, 1,2,4-trichloro-	180	C6H3Cl3	000120-82-1	98
3			Benzene, 1,2,3-trichloro-	180	C6H3Cl3	000087-61-6	98
4			Benzene, 1,3,5-trichloro-	180	C6H3Cl3	000108-70-3	97
5			Benzene, 1,2,3-trichloro-	180	C6H3Cl3	000087-61-6	96

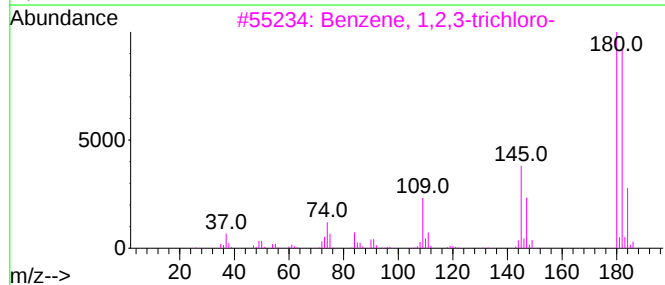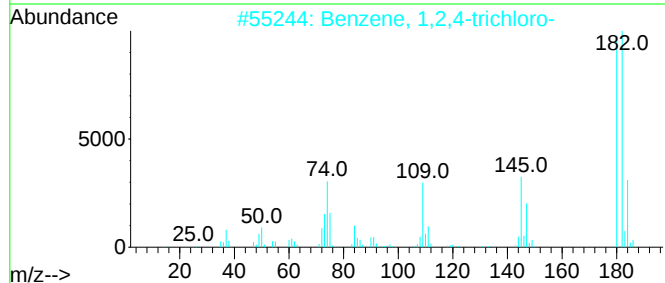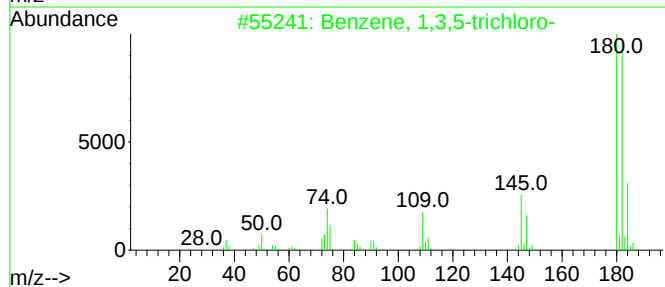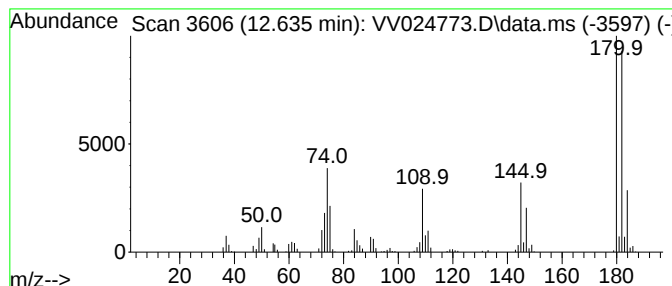

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022122\
Data File : VV024773.D
Acq On : 21 Feb 2022 14:02
Operator : SY/MD
Sample : N1623-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBD27

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzene, 1,3,5-...	12.644	3.7	ug/L	486251	3	11.246	664238	5.0