

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022122\
 Data File : VV024781.D
 Acq On : 21 Feb 2022 17:28
 Operator : SY/MD
 Sample : N1623-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBD30

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV024781.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	100	rVB	77791	79361	15.96%	1.941%
2	1.571	156	165	175	rBV	68874	79525	15.99%	1.945%
3	2.111	322	333	344	rBV	127993	185703	37.34%	4.543%
4	2.178	347	354	365	rVB	4329	9099	1.83%	0.223%
5	3.889	876	886	920	rBV	54468	164664	33.11%	4.028%
6	4.352	1013	1030	1066	rBV	87519	219902	44.21%	5.380%
7	5.050	1231	1247	1276	rBV2	200913	497388	100.00%	12.168%
8	5.619	1412	1424	1447	rBV	175458	354938	71.36%	8.683%
9	5.911	1505	1515	1529	rVB4	4282	9022	1.81%	0.221%
10	6.069	1552	1564	1592	rBV	115847	237428	47.73%	5.808%
11	6.989	1839	1850	1878	rBV	50482	95232	19.15%	2.330%
12	7.317	1940	1952	1971	rBV	237582	414705	83.38%	10.145%
13	7.625	2039	2048	2072	rBV	27819	50560	10.17%	1.237%
14	8.088	2182	2192	2237	rBV	219346	427517	85.95%	10.459%
15	8.850	2418	2429	2459	rBV	256599	425687	85.58%	10.414%
16	10.214	2840	2853	2869	rBV	69091	109297	21.97%	2.674%
17	11.246	3164	3174	3198	rBV	241241	376111	75.62%	9.201%
18	11.532	3256	3263	3278	rBV4	3810	7044	1.42%	0.172%
19	11.622	3278	3291	3315	rVB	216517	337810	67.92%	8.264%
20	13.519	3873	3881	3892	rBV3	4587	6685	1.34%	0.164%




Sum of corrected areas: 4087678

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022122\
Data File : VV024781.D
Acq On : 21 Feb 2022 17:28
Operator : SY/MD
Sample : N1623-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBD30

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

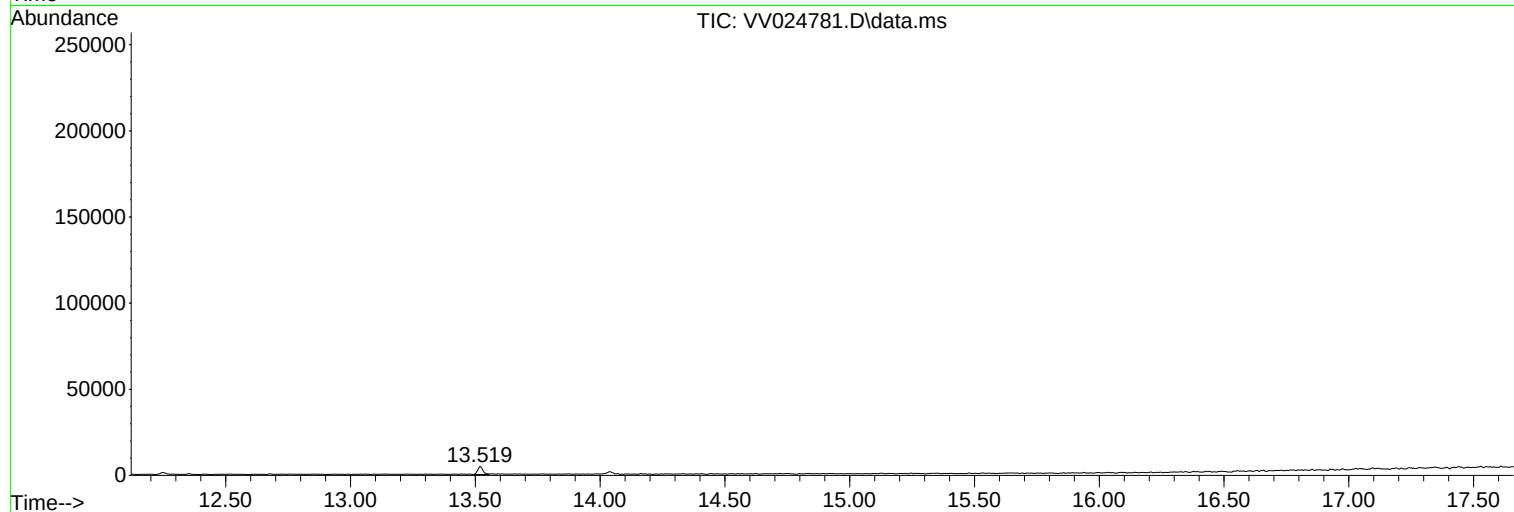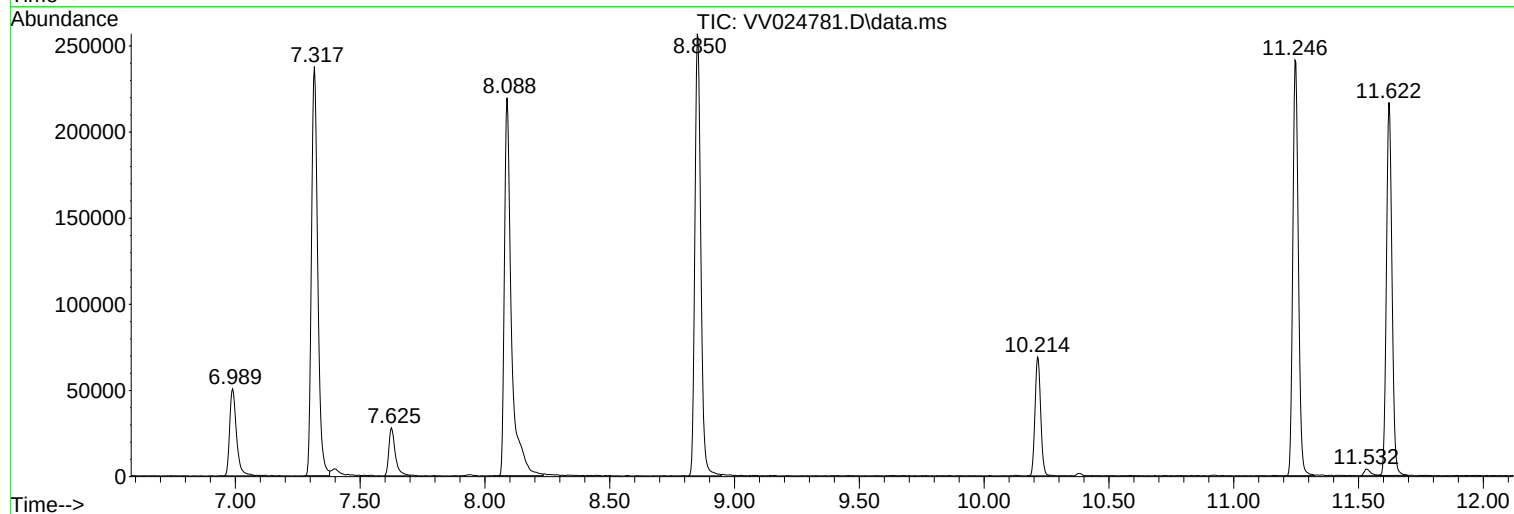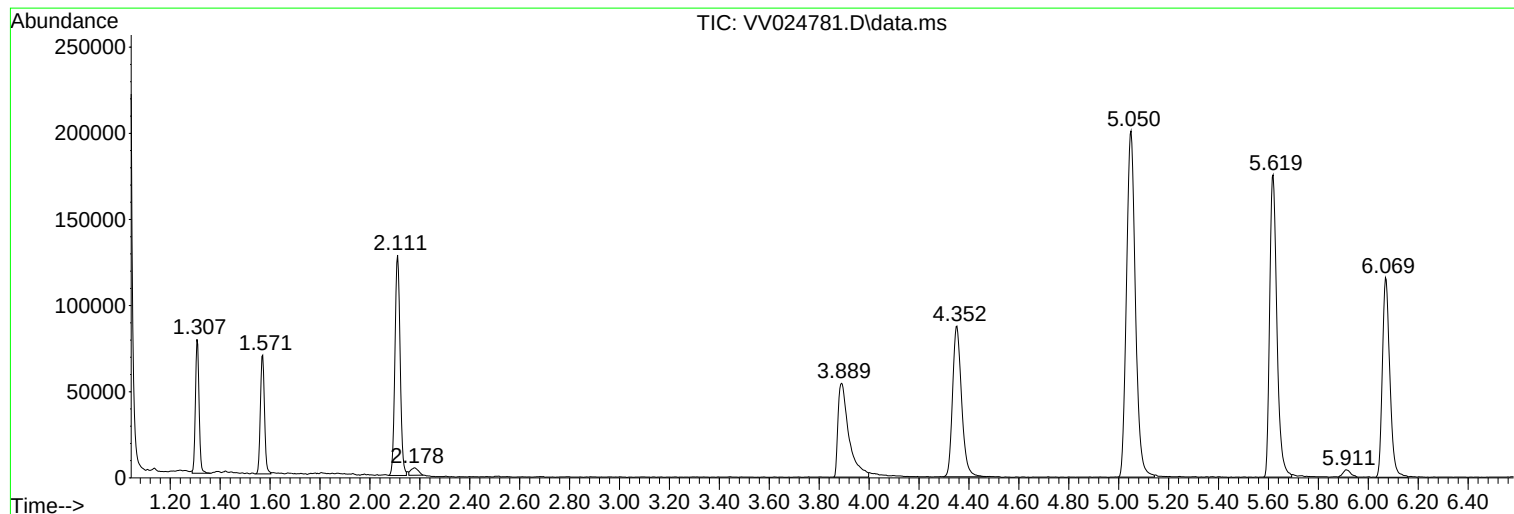

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022122\
Data File : VV024781.D
Acq On : 21 Feb 2022 17:28
Operator : SY/MD
Sample : N1623-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBD30

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022122\
Data File : VV024781.D
Acq On : 21 Feb 2022 17:28
Operator : SY/MD
Sample : N1623-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBD30

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc