

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022122\
 Data File : VV024785.D
 Acq On : 21 Feb 2022 19:02
 Operator : SY/MD
 Sample : N1623-13
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBD40

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV024785.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	98	rVB	76564	76914	15.90%	1.549%
2	1.417	103	117	126	rVB2	5419	7834	1.62%	0.158%
3	1.571	157	165	176	rBV	66861	75158	15.53%	1.514%
4	2.111	322	333	346	rBV	122331	179071	37.01%	3.607%
5	3.889	877	886	916	rBV	54446	161260	33.33%	3.249%
6	4.355	1012	1031	1061	rBV4	105801	361511	74.72%	7.283%
7	4.674	1120	1130	1142	rBV3	2653	5938	1.23%	0.120%
8	4.915	1191	1205	1221	rVB2	4334	10368	2.14%	0.209%
9	5.050	1230	1247	1277	rBV2	193823	483842	100.00%	9.747%
10	5.500	1374	1387	1400	rBV6	3871	8698	1.80%	0.175%
11	5.619	1411	1424	1454	rBV	183683	377950	78.11%	7.614%
12	5.912	1506	1515	1516	rBV5	4235	5151	1.06%	0.104%
13	6.069	1551	1564	1582	rBV	110793	231704	47.89%	4.668%
14	6.510	1687	1701	1723	rBV	134649	252426	52.17%	5.085%
15	6.989	1840	1850	1867	rBV	49990	92350	19.09%	1.860%
16	7.317	1940	1952	1968	rBV	224758	394422	81.52%	7.946%
17	7.394	1968	1976	2000	rVB	24810	47965	9.91%	0.966%
18	7.625	2038	2048	2070	rBV2	27172	50157	10.37%	1.010%
19	8.088	2182	2192	2226	rBV	212242	413964	85.56%	8.340%
20	8.246	2229	2241	2260	rVB	141551	239628	49.53%	4.827%
21	8.850	2418	2429	2451	rBV	274656	449916	92.99%	9.064%
22	9.021	2473	2482	2495	rVB2	6500	9972	2.06%	0.201%
23	9.143	2510	2520	2534	rBV	15670	26724	5.52%	0.538%
24	9.548	2638	2646	2663	rVB	8307	13817	2.86%	0.278%
25	9.731	2693	2703	2718	rVB2	29824	48621	10.05%	0.979%
26	10.214	2841	2853	2870	rBV	68378	107102	22.14%	2.158%
27	10.448	2917	2926	2946	rVB3	7081	15391	3.18%	0.310%
28	10.738	3010	3016	3029	rVB2	3932	5776	1.19%	0.116%
29	10.915	3061	3071	3085	rBV2	23209	35110	7.26%	0.707%
30	11.246	3164	3174	3193	rBV	271496	418458	86.49%	8.430%
31	11.336	3195	3202	3215	rVB	9125	13139	2.72%	0.265%
32	11.529	3253	3262	3270	rBV3	4941	7627	1.58%	0.154%
33	11.622	3280	3291	3312	rVB	209502	327439	67.67%	6.596%
34	14.014	4028	4035	4054	rVB6	4716	8458	1.75%	0.170%

Sum of corrected areas: 4963861




Instrument :
MSVOA_V
ClientSampleId :
GBD40

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022122\
Data File : VV024785.D
Acq On : 21 Feb 2022 19:02
Operator : SY/MD
Sample : N1623-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBD40

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

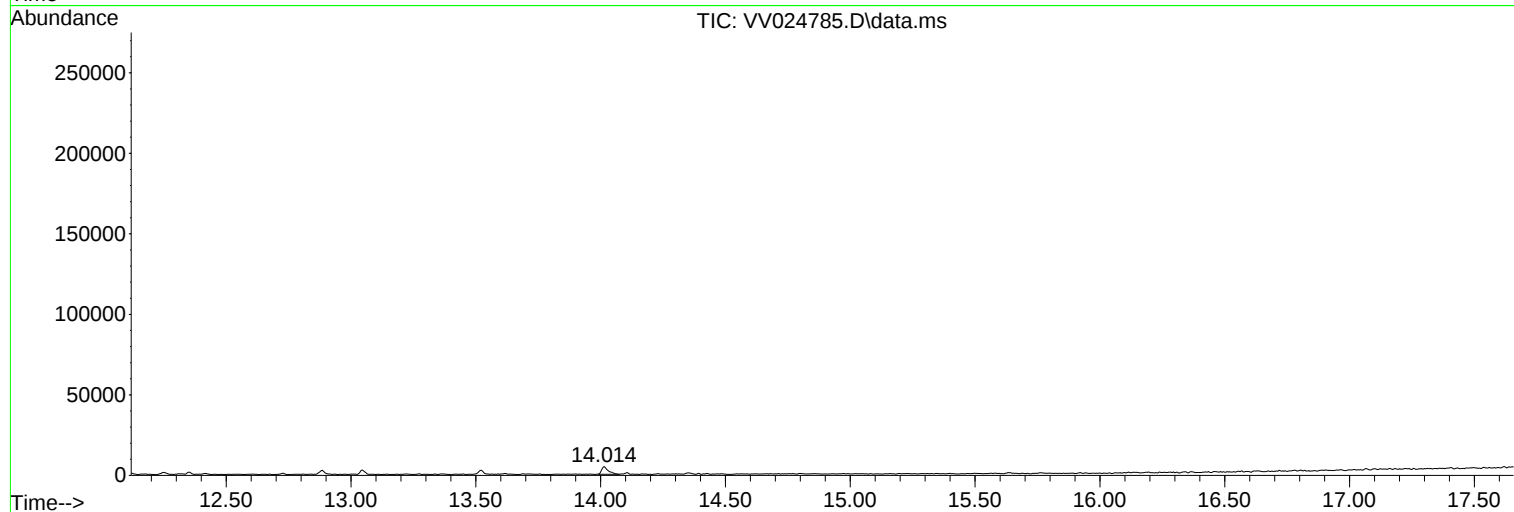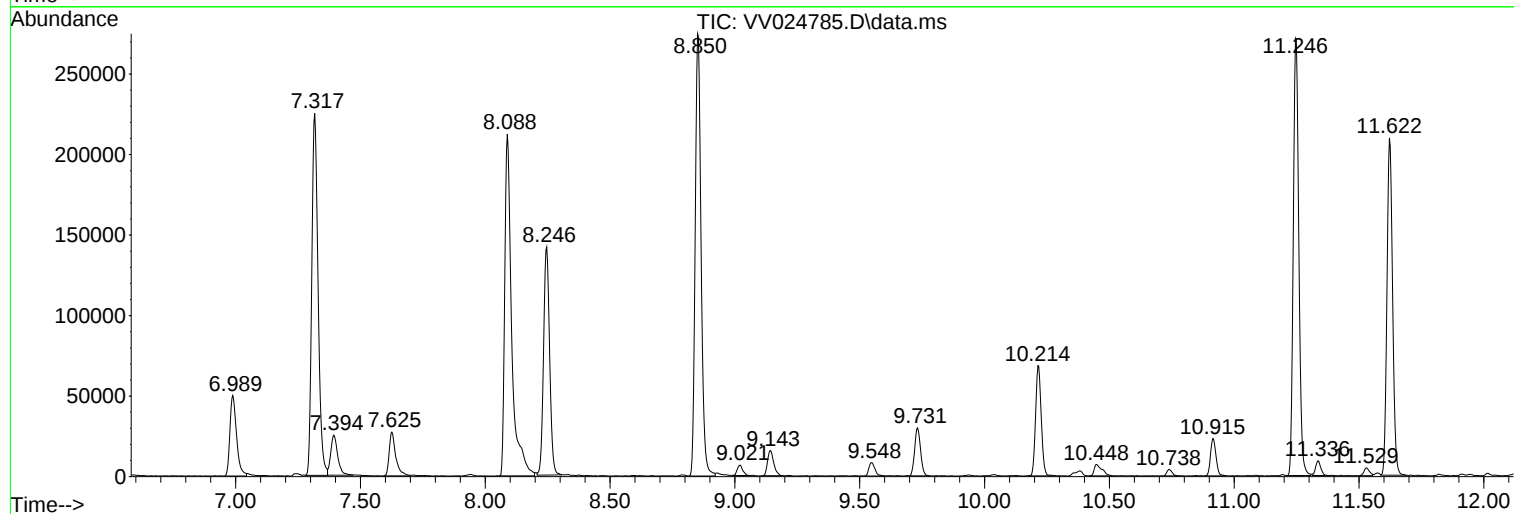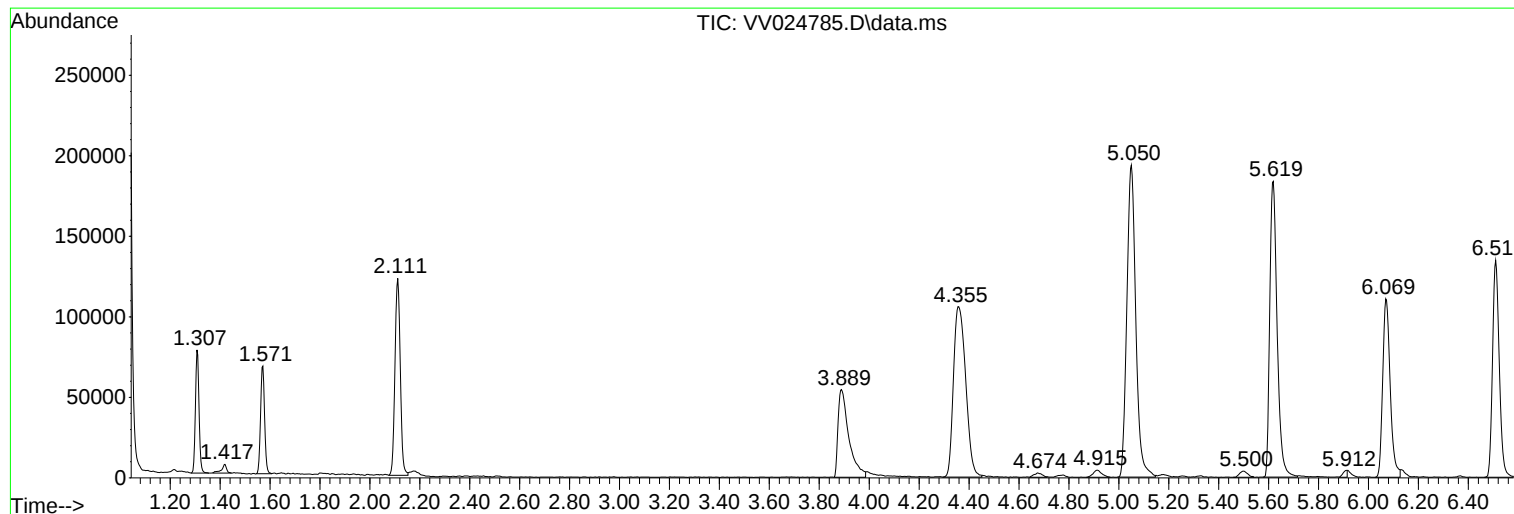

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022122\
Data File : VV024785.D
Acq On : 21 Feb 2022 19:02
Operator : SY/MD
Sample : N1623-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBD40

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022122\
Data File : VV024785.D
Acq On : 21 Feb 2022 19:02
Operator : SY/MD
Sample : N1623-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBD40

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
