

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022122\
 Data File : VV024786.D
 Acq On : 21 Feb 2022 19:25
 Operator : SY/MD
 Sample : N1623-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBD41

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV024786.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	94	rVB	76842	78033	16.25%	1.909%
2	1.568	156	164	176	rBV	67353	76527	15.93%	1.872%
3	2.111	321	333	349	rBV	121303	177130	36.88%	4.334%
4	3.886	871	885	929	rBV	54308	166257	34.61%	4.068%
5	4.349	1011	1029	1056	rBV	84141	212650	44.27%	5.203%
6	5.050	1231	1247	1280	rBV2	190401	480328	100.00%	11.753%
7	5.616	1409	1423	1459	rBV	188940	379806	79.07%	9.293%
8	5.912	1506	1515	1530	rBV4	4814	9545	1.99%	0.234%
9	6.069	1552	1564	1597	rBV	111252	228898	47.65%	5.601%
10	6.989	1837	1850	1877	rBV	48143	91943	19.14%	2.250%
11	7.317	1940	1952	1972	rBV	226510	396476	82.54%	9.701%
12	7.400	1974	1978	1996	rVB6	3852	6729	1.40%	0.165%
13	7.625	2039	2048	2067	rBV2	26547	47633	9.92%	1.165%
14	8.088	2182	2192	2240	rBV	212598	418108	87.05%	10.230%
15	8.850	2418	2429	2465	rBV	276804	451444	93.99%	11.046%
16	10.214	2843	2853	2869	rBV2	67687	105575	21.98%	2.583%
17	11.249	3163	3175	3191	rBV	262090	410287	85.42%	10.039%
18	11.532	3252	3263	3277	rBV2	9540	17071	3.55%	0.418%
19	11.622	3280	3291	3313	rVB	210601	326133	67.90%	7.980%
20	17.345	5067	5071	5078	rVB	8146	6352	1.32%	0.155%




Sum of corrected areas: 4086925

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022122\
Data File : VV024786.D
Acq On : 21 Feb 2022 19:25
Operator : SY/MD
Sample : N1623-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBD41

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

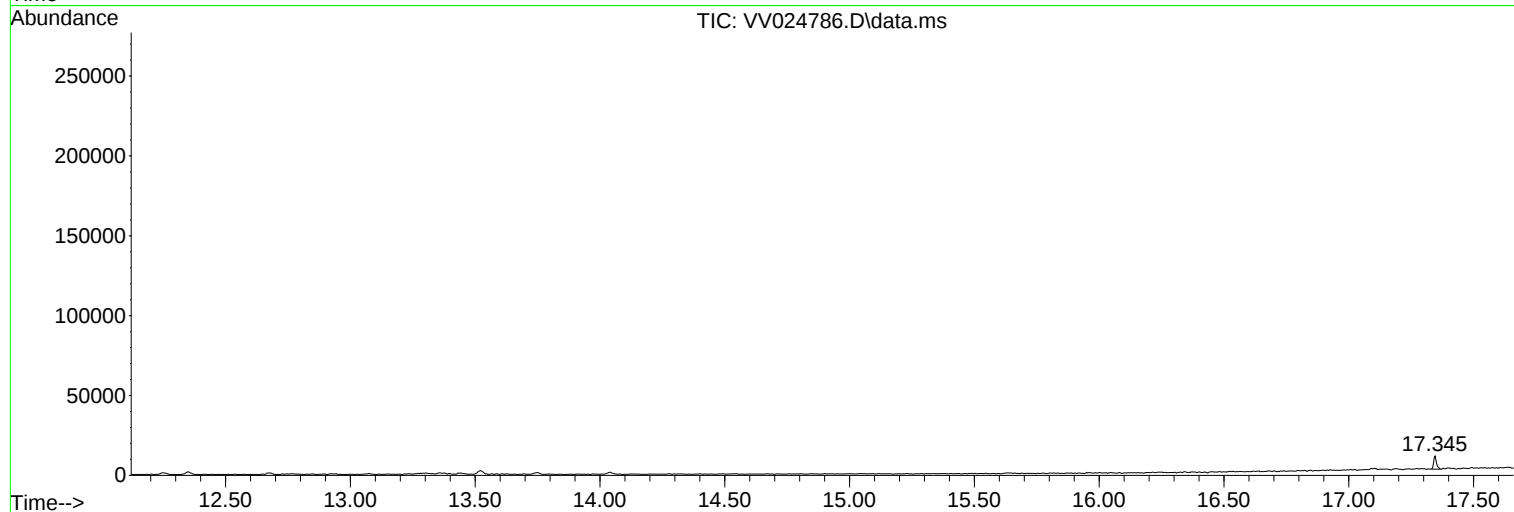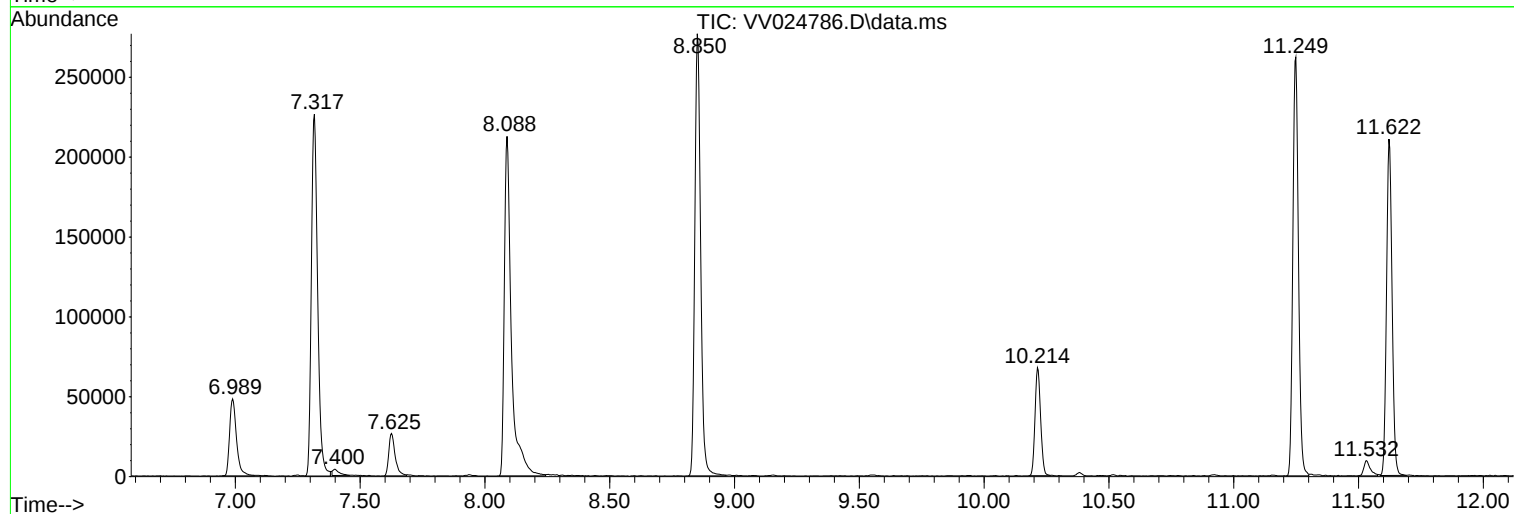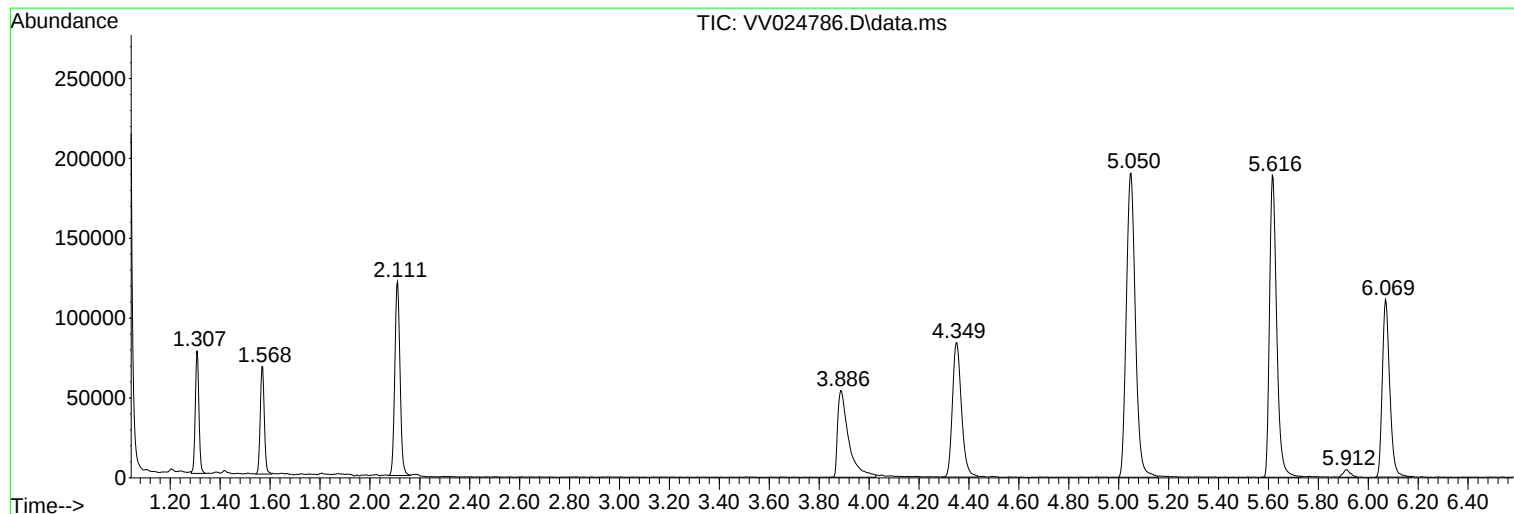

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022122\
Data File : VV024786.D
Acq On : 21 Feb 2022 19:25
Operator : SY/MD
Sample : N1623-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBD41

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022122\
Data File : VV024786.D
Acq On : 21 Feb 2022 19:25
Operator : SY/MD
Sample : N1623-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBD41

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc