
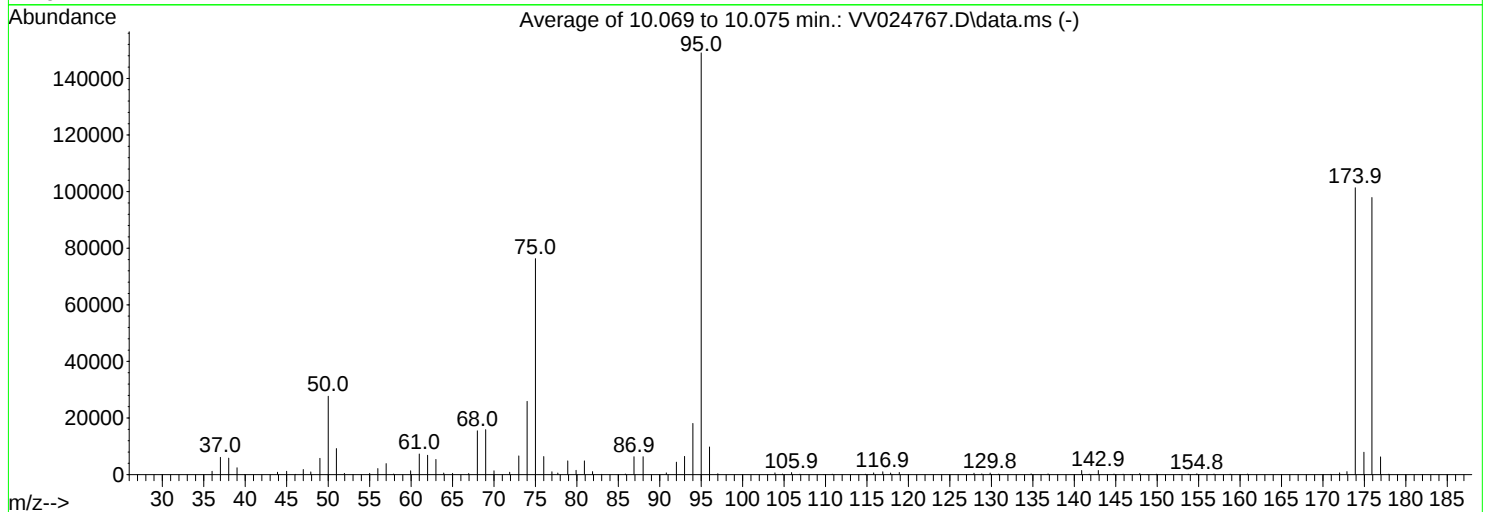


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022122\
 Data File : VV024767.D
 Acq On : 21 Feb 2022 09:27
 Operator : SY/MD
 Sample : BFB274
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB274

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Fri Feb 25 03:28:05 2022

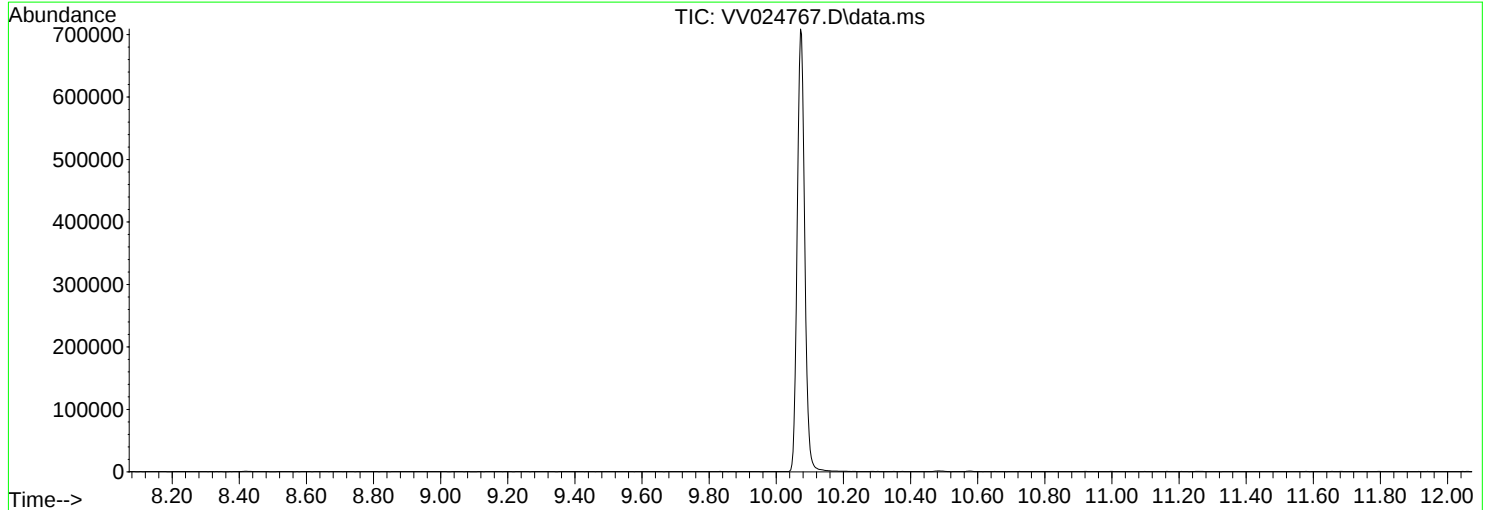

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	27699	PASS
75	95	30	80	51.2	76349	PASS
95	95	100	100	100.0	149035	PASS
96	95	5	9	6.6	9793	PASS
173	174	0.00	2	1.1	1106	PASS
174	95	50	120	68.0	101341	PASS
175	174	5	9	7.8	7892	PASS
176	174	95	105	96.6	97925	PASS
177	176	5	10	6.4	6287	PASS

m/z	Abundance
36.00	1210.0
37.00	6032.0
38.00	5636.0
39.00	2342.0
40.00	180.0
44.00	1070.0
45.00	1120.0
46.20	114.0
47.00	1735.0
47.90	952.0
49.00	5522.0
50.00	26712.0
51.00	9101.0
52.00	442.0
55.00	441.0
56.00	2090.0
57.00	3742.0
57.90	212.0
60.00	1377.0
61.00	7022.0
62.00	6702.0
63.00	5231.0
63.90	514.0
65.00	451.0
66.90	346.0
68.00	14784.0
69.00	15460.0
70.00	1247.0
71.90	788.0
73.00	6543.0
74.00	25080.0
75.00	73032.0
76.00	6213.0
77.00	901.0
77.70	592.0
78.90	4664.0
79.90	1401.0
80.90	4678.0
81.90	1038.0
85.80	218.0
86.90	5854.0
88.00	5818.0
90.80	621.0
92.00	4051.0
93.00	6077.0
94.00	16944.0
95.00	140864.0
96.00	9652.0
97.00	354.0
103.90	603.0
104.80	179.0
105.90	763.0
106.90	153.0
110.80	154.0
114.80	179.0
115.80	580.0
116.90	981.0
117.90	523.0
118.90	621.0
127.90	431.0
128.80	256.0
129.80	524.0
130.90	196.0
134.90	287.0
136.90	271.0
140.00	107.0
140.90	1422.0
141.80	213.0
142.90	1382.0
144.80	186.0
145.90	181.0
147.90	380.0
150.00	121.0
152.70	114.0
153.80	163.0
154.80	366.0
156.80	190.0
158.80	128.0
160.90	221.0
170.00	103.0
170.90	107.0
172.00	532.0
172.90	1058.0
173.90	93568.0
174.90	7197.0
175.90	90520.0
176.90	5888.0
178.00	144.0

Instrument :
MSVOA_V
ClientSampleId :
BFB274

Scan 2796 (10.030 min): VV024767.D\data.ms
BFB274

m/z	Abundance
39.90	161.0
43.90	330.0

Instrument :
MSVOA_V
ClientSampleId :
BFB274

m/z	Abundance
36.00	1216.0
37.00	6332.0
38.00	6023.0
39.00	2528.0
39.90	198.0
44.00	1195.0
45.00	1208.0
46.00	116.0
47.00	1848.0
47.90	1011.0
49.00	5971.0
50.00	28624.0
51.00	9603.0
52.00	494.0
53.00	105.0
55.00	467.0
56.00	2261.0
57.00	3962.0
57.90	212.0
59.90	1412.0
61.00	7638.0
62.00	7058.0
63.00	5560.0
63.90	601.0
65.00	454.0
67.00	410.0
68.00	15973.0
69.00	16504.0
70.00	1394.0
71.90	843.0
73.00	6841.0
74.00	26712.0
75.00	79024.0
76.00	6616.0
77.00	1066.0
77.70	574.0
78.90	5017.0
79.90	1553.0
80.90	5064.0
81.90	1078.0
83.00	129.0
85.90	226.0
86.90	6554.0
88.00	6591.0
90.80	661.0
92.00	4572.0
93.00	6630.0
94.00	18592.0
95.00	153984.0
96.00	10031.0
97.00	331.0
103.90	630.0
104.80	217.0
105.90	793.0
106.90	164.0
109.80	130.0
110.80	184.0
114.80	184.0
115.80	625.0
116.90	1102.0
117.90	553.0
118.90	808.0
127.90	497.0
128.80	269.0
129.90	584.0
130.90	218.0
134.80	293.0
136.90	317.0
140.90	1485.0
141.80	197.0
142.90	1515.0
144.80	213.0
145.90	157.0
146.80	116.0
147.90	443.0
149.90	151.0
152.80	109.0
153.80	136.0
154.80	386.0
156.90	204.0
158.80	158.0
160.90	217.0
170.10	103.0
170.90	132.0
172.00	661.0
172.90	1141.0
173.90	104776.0
174.90	8166.0
175.90	101160.0
177.00	6494.0
177.90	151.0

Instrument :
MSVOA_V
ClientSampleId :
BFB274

m/z	Abundance
36.00	1093.0
37.00	6028.0
38.00	5809.0
39.00	2427.0
39.90	234.0
43.90	1243.0
45.00	1208.0
46.00	134.0
47.00	1790.0
47.90	908.0
49.00	5846.0
50.00	27760.0
51.00	8941.0
51.90	516.0
55.00	454.0
56.00	2182.0
57.00	3939.0
57.90	196.0
59.90	1370.0
61.00	7322.0
62.00	6722.0
63.00	5350.0
64.00	645.0
65.00	410.0
67.00	403.0
68.00	15681.0
69.00	15718.0
70.00	1376.0
71.90	849.0
73.00	6533.0
74.00	25848.0
75.00	76992.0
76.00	6403.0
77.00	1106.0
77.70	476.0
78.90	4924.0
79.90	1571.0
80.90	4851.0
81.90	1149.0
83.00	164.0
85.80	192.0
86.90	6675.0
88.00	6552.0
90.80	637.0
92.00	4649.0
93.00	6701.0
94.00	18736.0
95.00	152256.0
96.00	9696.0
97.00	279.0
103.90	607.0
104.80	249.0
105.90	721.0
106.90	149.0
109.80	107.0
110.80	172.0
114.80	190.0
115.80	599.0
116.90	1034.0
117.80	555.0
118.90	881.0
127.90	543.0
128.90	283.0
129.90	578.0
130.90	229.0
134.70	302.0
136.80	310.0
140.90	1457.0
141.80	166.0
142.90	1517.0
144.80	209.0
145.90	128.0
146.80	137.0
147.90	403.0
148.80	101.0
149.80	160.0
153.70	136.0
154.80	340.0
156.90	208.0
158.80	199.0
160.90	167.0
171.00	127.0
172.00	678.0
172.90	1119.0
173.90	105680.0
175.00	8313.0
175.90	102096.0
177.00	6478.0
178.00	168.0

Instrument :
MSVOA_V
ClientSampleId :
BFB274