


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV022219\
 Data File : VV009327.D
 Acq On : 22 Feb 2019 13:07
 Operator : SY/MD
 Sample : BFB65
 Misc : 5.00G/10ML/MSVOA_V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB65

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM022019S.M
 Title : VOC Analysis
 Last Update : Sat Feb 23 00:37:16 2019

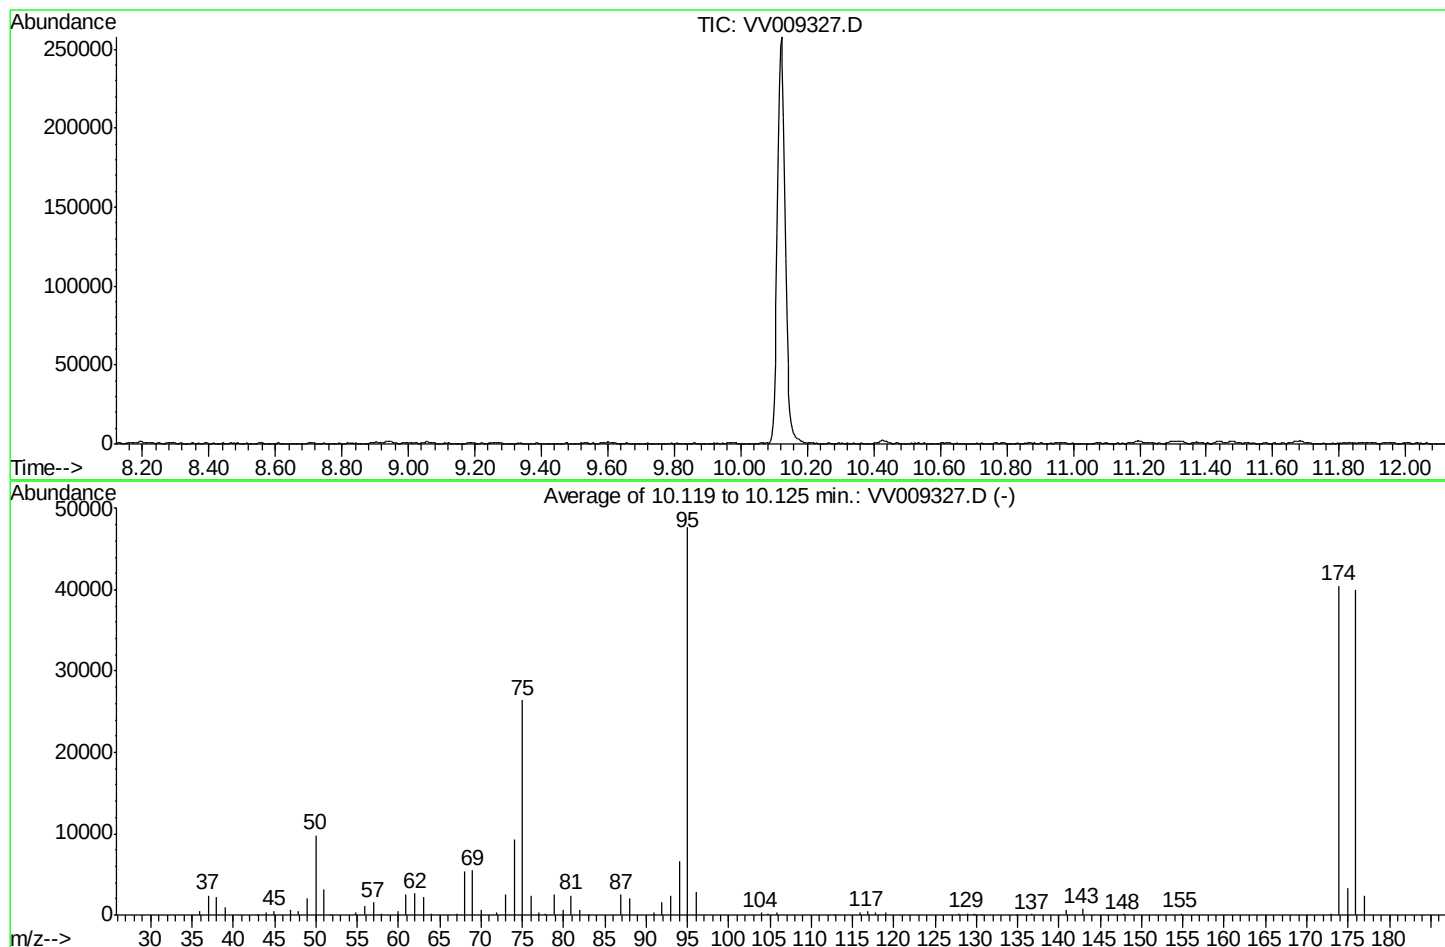

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.5	9793	PASS
75	95	30	80	55.3	26384	PASS
95	95	100	100	100.0	47685	PASS
96	95	5	9	6.0	2882	PASS
173	174	0.00	2	0.5	191	PASS
174	95	50	120	85.0	40546	PASS
175	174	5	9	8.2	3316	PASS
176	174	95	101	98.5	39944	PASS
177	176	5	9	5.9	2362	PASS

m/z	Abundance
35.90	450.0
37.00	2385.0
38.00	2263.0
39.00	955.0
42.90	141.0
44.00	674.0
45.00	470.0
46.90	754.0
47.90	425.0
49.00	2140.0
50.00	10059.0
51.00	3031.0
54.80	277.0
55.90	1184.0
57.00	1576.0
57.90	108.0
59.90	445.0
61.00	2487.0
62.00	2659.0
63.00	2140.0
64.00	218.0
67.00	145.0
68.00	5559.0
69.00	5718.0
70.00	626.0
72.00	388.0
73.00	2748.0
74.00	9599.0
75.00	26768.0
76.00	2472.0
77.00	301.0
77.80	296.0
78.90	2570.0
79.90	662.0
80.90	2364.0
81.90	583.0
86.90	2453.0
88.00	2128.0
90.90	310.0
92.00	1617.0
93.00	2212.0
94.00	6636.0
95.00	48664.0
96.00	3016.0
103.90	288.0
104.80	138.0
105.80	235.0
115.80	228.0
116.80	389.0
117.80	271.0
118.90	291.0
127.80	144.0
128.90	183.0
129.70	206.0
134.80	127.0
136.70	138.0
140.90	658.0
142.80	741.0
147.80	160.0
154.80	165.0
173.00	574.0
173.90	40184.0
174.90	3274.0
175.90	38864.0
176.90	2439.0

Instrument :
MSVOA_V
ClientSampleId :
BFB65

m/z	Abundance
35.90	476.0
37.00	2465.0
38.00	2356.0
39.00	958.0
39.90	102.0
42.90	143.0
44.00	655.0
44.90	509.0
46.90	691.0
47.90	450.0
49.00	2018.0
50.00	10038.0
51.00	3220.0
54.80	263.0
55.90	1060.0
57.00	1623.0
57.90	115.0
60.00	444.0
61.00	2559.0
62.00	2666.0
63.00	2209.0
64.00	220.0
67.00	183.0
68.00	5569.0
69.00	5599.0
70.00	579.0
72.00	362.0
73.00	2602.0
74.00	9651.0
75.00	27232.0
76.00	2450.0
77.00	351.0
77.80	240.0
78.90	2630.0
79.90	633.0
80.90	2506.0
81.90	622.0
83.00	103.0
87.00	2682.0
87.90	2092.0
90.90	267.0
92.00	1597.0
93.00	2451.0
94.00	6818.0
95.00	48984.0
96.00	2951.0
103.90	309.0
104.80	119.0
105.90	270.0
112.80	102.0
115.90	262.0
116.80	441.0
117.70	254.0
119.00	266.0
127.80	110.0
128.90	201.0
129.70	229.0
130.70	114.0
134.90	103.0
136.80	124.0
140.90	724.0
142.80	762.0
147.80	150.0
154.80	180.0
173.90	41640.0
174.90	3403.0
175.90	41152.0
176.90	2374.0

Instrument :
MSVOA_V
ClientSampleId :
BFB65

m/z	Abundance
35.90	507.0
37.00	2286.0
38.00	2167.0
39.00	891.0
42.90	137.0
44.00	617.0
44.90	539.0
47.00	505.0
47.90	412.0
49.00	1788.0
50.00	9283.0
51.00	3008.0
51.70	142.0
54.80	215.0
55.90	887.0
57.00	1523.0
57.90	105.0
60.00	419.0
60.90	2444.0
62.00	2552.0
63.00	2064.0
64.00	203.0
67.00	193.0
68.00	5060.0
69.00	5071.0
70.00	491.0
71.90	297.0
73.00	2187.0
74.00	8757.0
75.00	25152.0
76.00	2111.0
77.00	357.0
77.80	172.0
78.90	2441.0
80.00	623.0
80.90	2424.0
81.90	624.0
87.00	2405.0
87.90	1826.0
91.00	203.0
91.90	1496.0
93.00	2399.0
94.00	6471.0
95.00	45408.0
96.00	2681.0
103.90	316.0
105.80	263.0
112.80	102.0
115.90	247.0
116.80	421.0
117.70	223.0
119.00	276.0
127.90	116.0
128.90	181.0
129.90	226.0
130.70	114.0
136.80	128.0
140.90	693.0
142.90	679.0
147.80	141.0
154.80	172.0
173.90	39816.0
174.90	3272.0
175.90	39816.0
176.90	2273.0

Instrument :
MSVOA_V
ClientSampleId :
BFB65

m/z	Abundance
39.90	107.0
42.90	103.0
44.00	265.0

Instrument :
MSVOA_V
ClientSampleId :
BFB65