

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022222\
 Data File : VV024791.D
 Acq On : 22 Feb 2022 12:35
 Operator : SY/MD
 Sample : VV0222WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK310

Quant Time: Feb 23 01:06:22 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Feb 22 03:27:30 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	160642	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	143905	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	62918	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	71913	5.278	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	105.600%	
7) Chloroethane-d5	1.568	69	56399	5.046	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	101.000%	
11) 1,1-Dichloroethene-d2	2.108	63	90047	3.606	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	72.200%	
20) 2-Butanone-d5	3.886	46	97021	49.851	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	99.700%	
24) Chloroform-d	4.346	84	102873	4.839	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	96.800%	
26) 1,2-Dichloroethane-d4	5.030	65	47321	4.993	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	99.800%	
32) Benzene-d6	5.047	84	221699	5.340	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	106.800%	
36) 1,2-Dichloropropane-d6	6.066	67	66129	5.413	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	108.200%	
41) Toluene-d8	7.313	98	193424	5.127	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	102.600%	
43) trans-1,3-Dichloroprop...	7.622	79	20147	4.950	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	99.000%	
46) 2-Hexanone-d5	8.085	63	71205	44.462	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	88.920%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	35886	4.874	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	97.400%	
66) 1,2-Dichlorobenzene-d4	11.622	152	55929	5.137	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	102.800%	
Target Compounds					Qvalue	
25) Chloroform	4.375	83	3284	0.141	ug/L	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022222\
Data File : VV024791.D
Acq On : 22 Feb 2022 12:35
Operator : SY/MD
Sample : VV02222WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK310

Quant Time: Feb 23 01:06:22 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Feb 22 03:27:30 2022
Response via : Initial Calibration

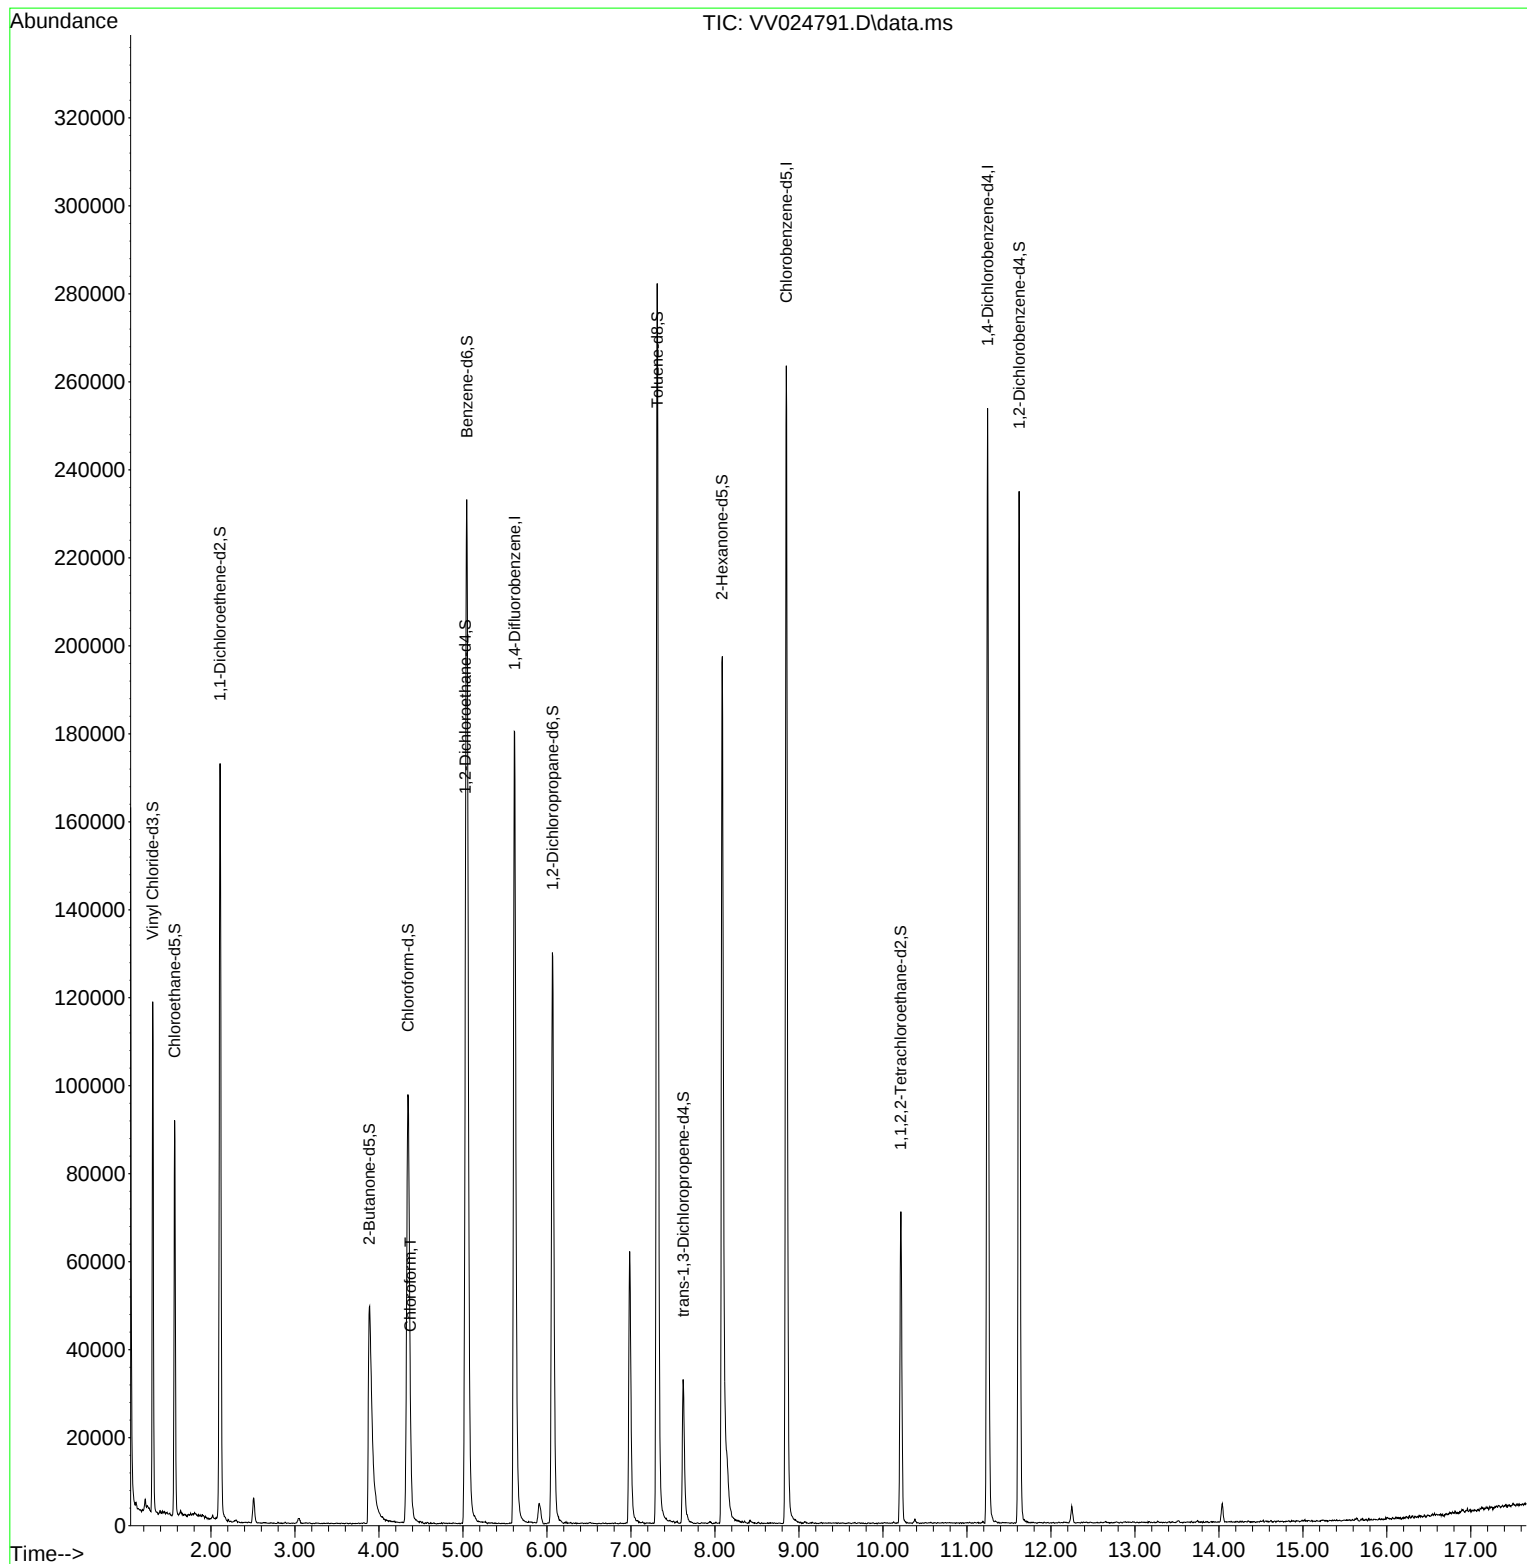

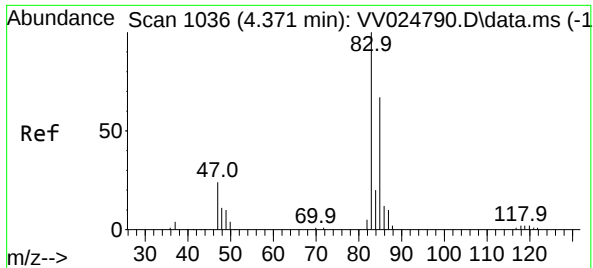

#25
 Chloroform
 Concen: 0.141 ug/L
 RT: 4.375 min Scan# 10
 Delta R.T. 0.003 min
 Lab File: VV024791.D
 Acq: 22 Feb 2022 12:35

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK310

Tgt Ion: 83 Resp: 3284
 Ion Ratio Lower Upper
 83 100
 85 77.6 45.5 84.5

