

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW022222\
 Data File : VW024794.D
 Acq On : 22 Feb 2022 13:59
 Operator : SY/MD
 Sample : N1623-18
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBD45

Quant Time: Feb 23 01:07:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Feb 22 03:27:30 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	156063	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	146468	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	63773	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	43100	3.256	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	65.200%	
7) Chloroethane-d5	1.568	69	40111	3.694	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	73.800%	
11) 1,1-Dichloroethene-d2	2.108	63	60108	2.478	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	49.600%#	
20) 2-Butanone-d5	3.892	46	90734	47.988	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	95.980%	
24) Chloroform-d	4.352	84	84654	4.098	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	82.000%	
26) 1,2-Dichloroethane-d4	5.034	65	40020	4.347	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	87.000%	
32) Benzene-d6	5.050	84	171967	4.070	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	81.400%	
36) 1,2-Dichloropropane-d6	6.069	67	53896	4.334	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	86.600%	
41) Toluene-d8	7.317	98	142603	3.714	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	74.200%	
43) trans-1,3-Dichloroprop...	7.628	79	15465	3.733	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	74.600%	
46) 2-Hexanone-d5	8.088	63	69320	42.528	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	85.060%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	32385	4.321	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	86.400%	
66) 1,2-Dichlorobenzene-d4	11.622	152	47677	4.321	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	86.400%	
Target Compounds					Qvalue	
25) Chloroform	4.384	83	1665	0.073	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022222\
Data File : VV024794.D
Acq On : 22 Feb 2022 13:59
Operator : SY/MD
Sample : N1623-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBD45

Quant Time: Feb 23 01:07:05 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Feb 22 03:27:30 2022
Response via : Initial Calibration

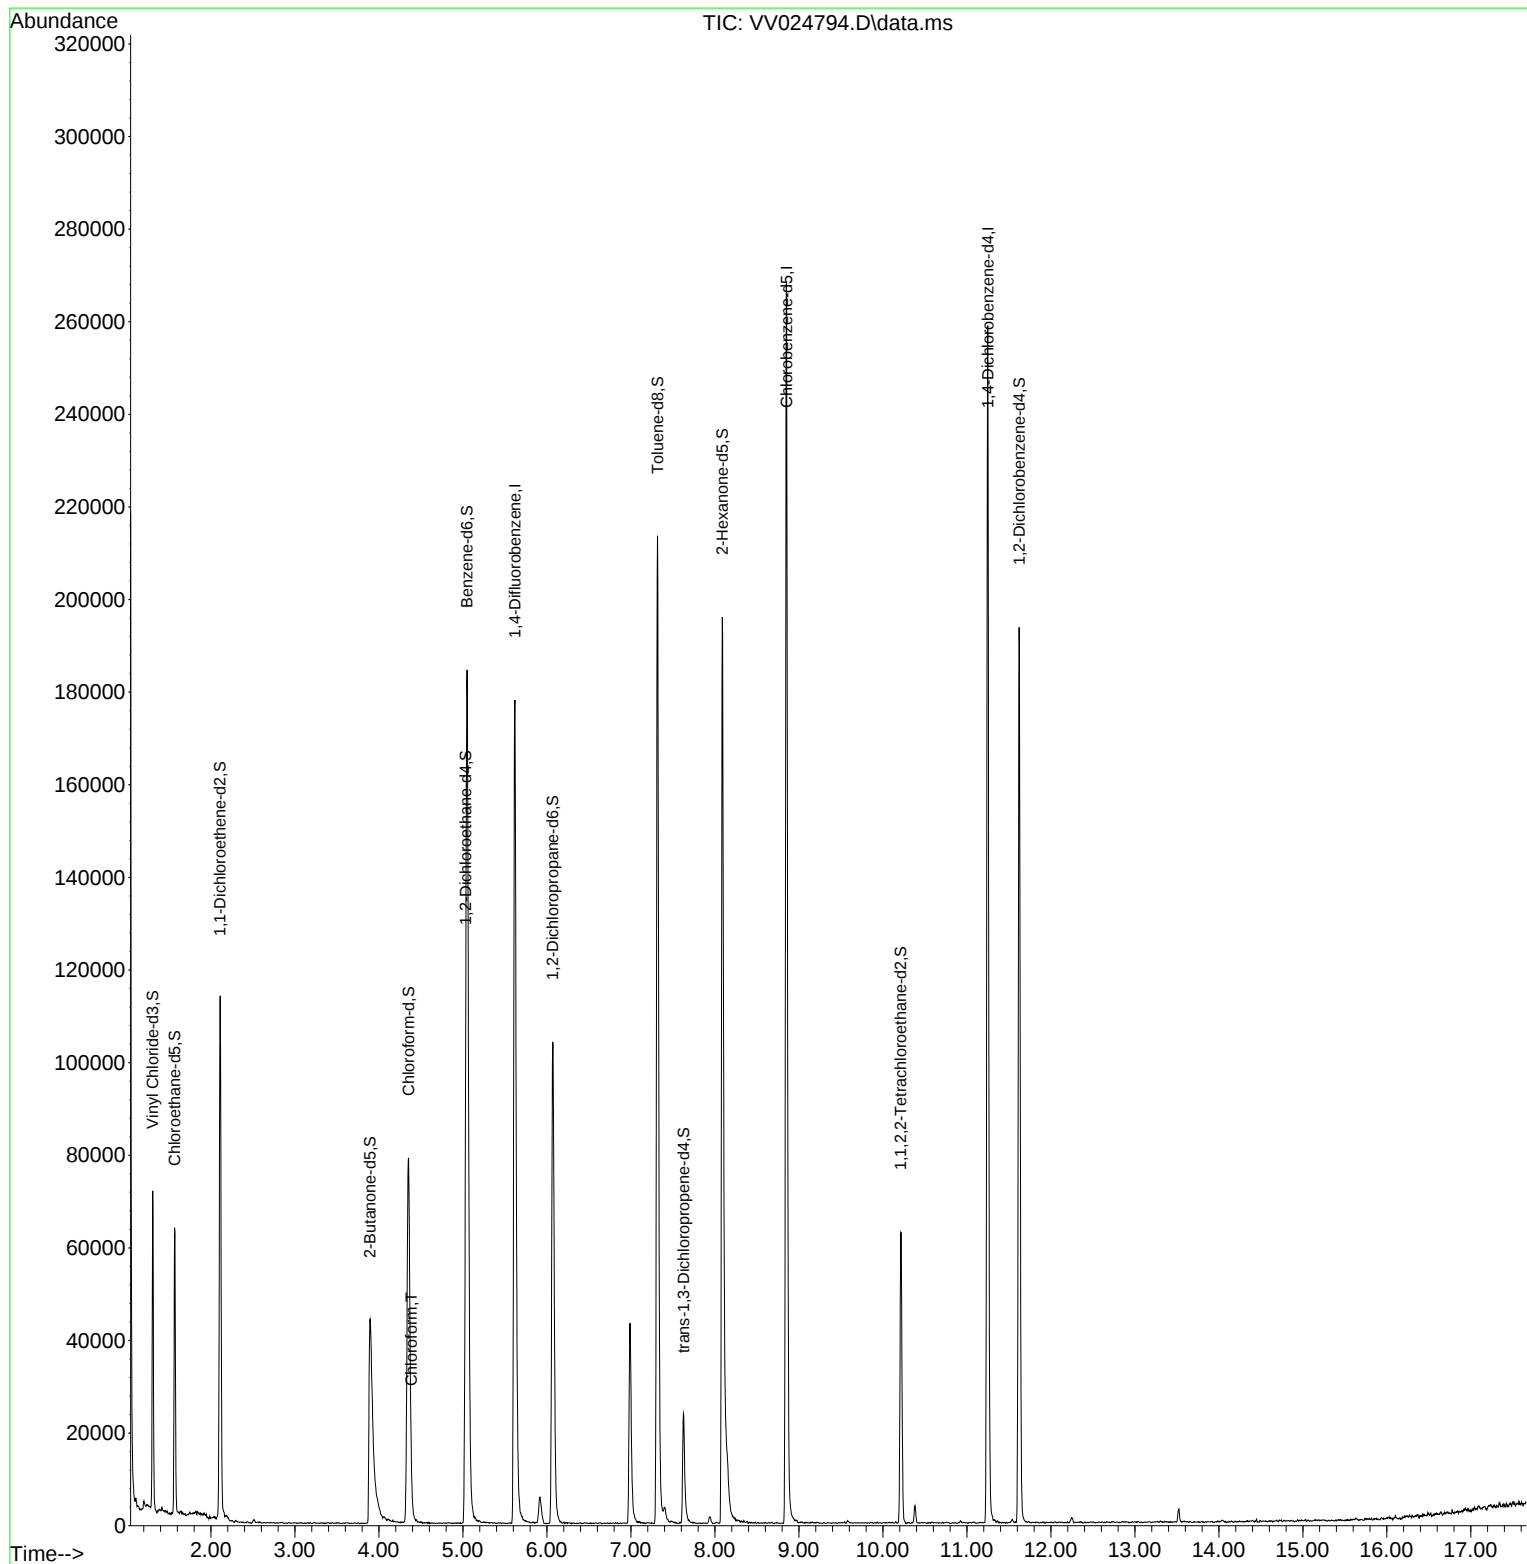

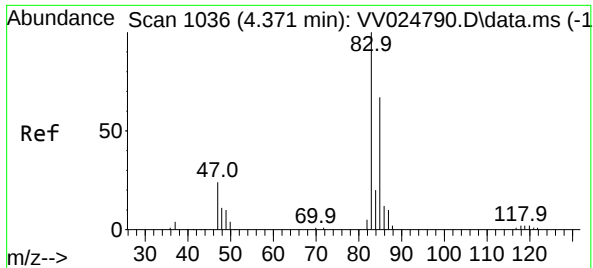

#25
 Chloroform
 Concen: 0.073 ug/L
 RT: 4.384 min Scan# 10
 Delta R.T. 0.013 min
 Lab File: VV024794.D
 Acq: 22 Feb 2022 13:59

Instrument :
 MSVOA_V
 ClientSampleId :
 GBD45

Tgt Ion: 83 Resp: 1665
 Ion Ratio Lower Upper
 83 100
 85 64.9 45.5 84.5

