

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022222\
 Data File : VV024791.D
 Acq On : 22 Feb 2022 12:35
 Operator : SY/MD
 Sample : VV0222WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK310

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV024791.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	98	rVB	116034	116056	20.18%	2.597%
2	1.568	156	164	175	rBV	89629	99985	17.38%	2.237%
3	2.108	320	332	357	rVB	172126	251206	43.67%	5.621%
4	2.506	447	456	470	rVB2	5701	9353	1.63%	0.209%
5	3.889	875	886	929	rBV	49349	160150	27.84%	3.584%
6	4.346	1011	1028	1056	rBV	97339	246658	42.88%	5.519%
7	5.043	1230	1245	1272	rBV2	232680	575199	100.00%	12.871%
8	5.612	1411	1422	1455	rBV	179931	364148	63.31%	8.148%
9	5.908	1504	1514	1532	rVB5	4670	11074	1.93%	0.248%
10	6.066	1550	1563	1589	rBV	129656	265739	46.20%	5.946%
11	6.985	1839	1849	1874	rBV	61719	111921	19.46%	2.504%
12	7.313	1939	1951	1983	rBV	281799	498583	86.68%	11.156%
13	7.622	2038	2047	2061	rBV2	32642	57702	10.03%	1.291%
14	8.088	2182	2192	2234	rBV	197057	391937	68.14%	8.770%
15	8.850	2415	2429	2456	rBV	263194	430958	74.92%	9.643%
16	10.214	2842	2853	2869	rBV	70779	112144	19.50%	2.509%
17	11.246	3164	3174	3199	rBV	253448	392802	68.29%	8.789%
18	11.622	3277	3291	3308	rBV	234568	361005	62.76%	8.078%
19	12.249	3475	3486	3495	rBV	3816	5876	1.02%	0.131%
20	14.040	4033	4043	4052	rBV	4246	6506	1.13%	0.146%




Sum of corrected areas: 4469002

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022222\
Data File : VV024791.D
Acq On : 22 Feb 2022 12:35
Operator : SY/MD
Sample : VV02222WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK310

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

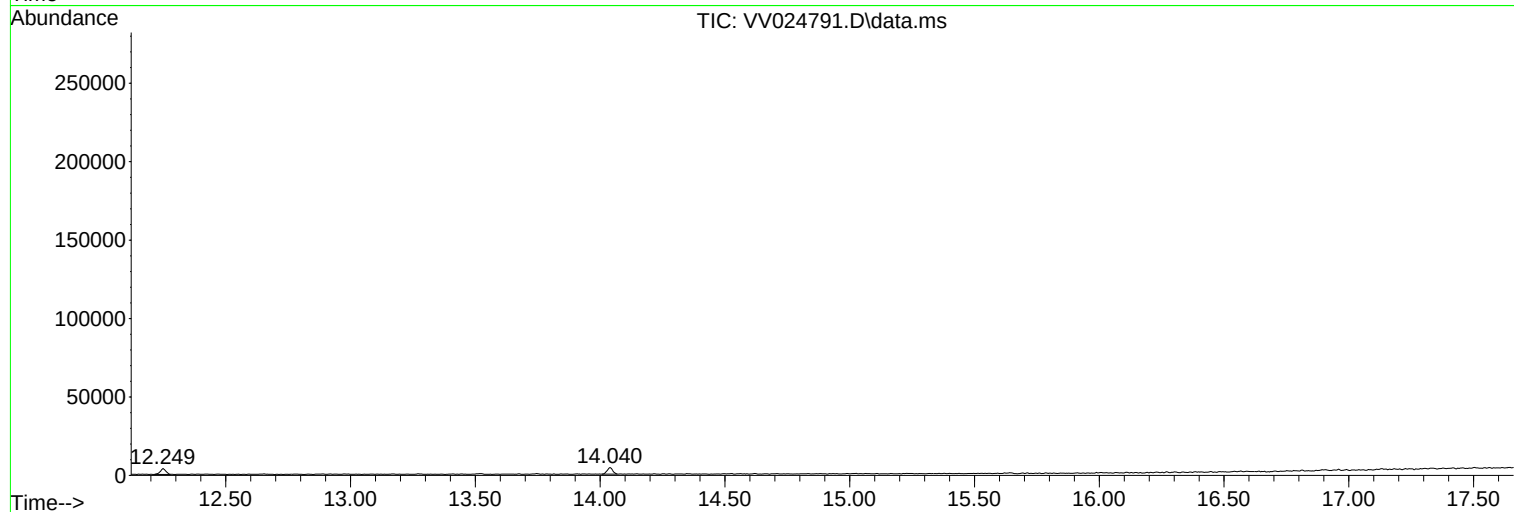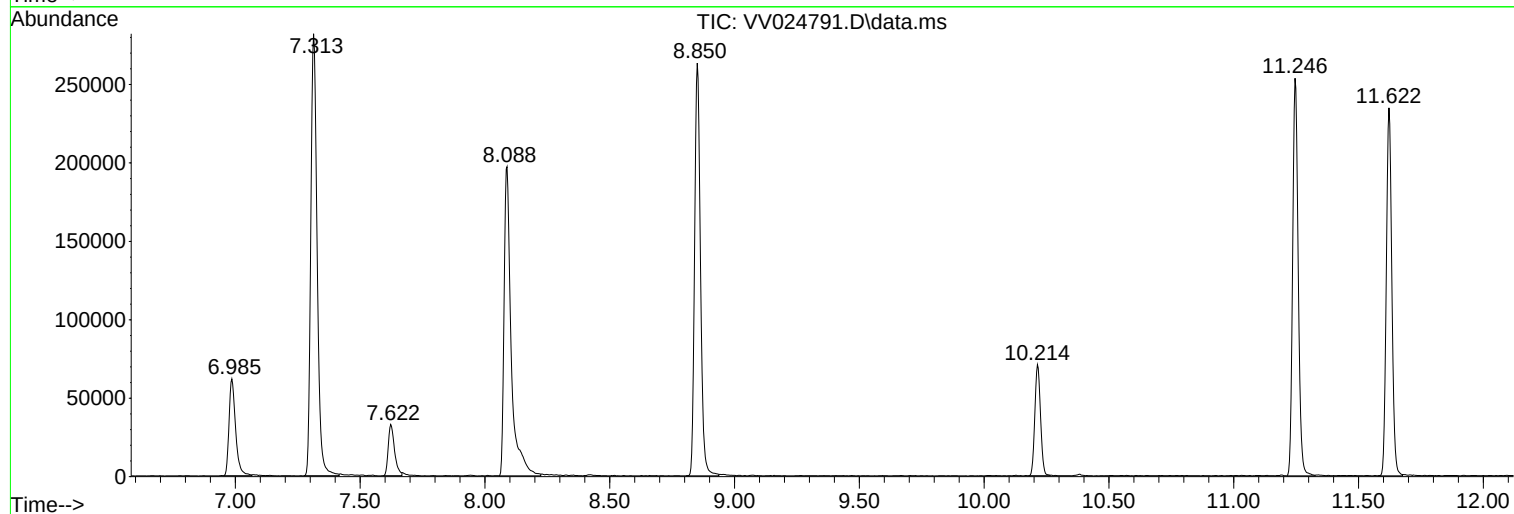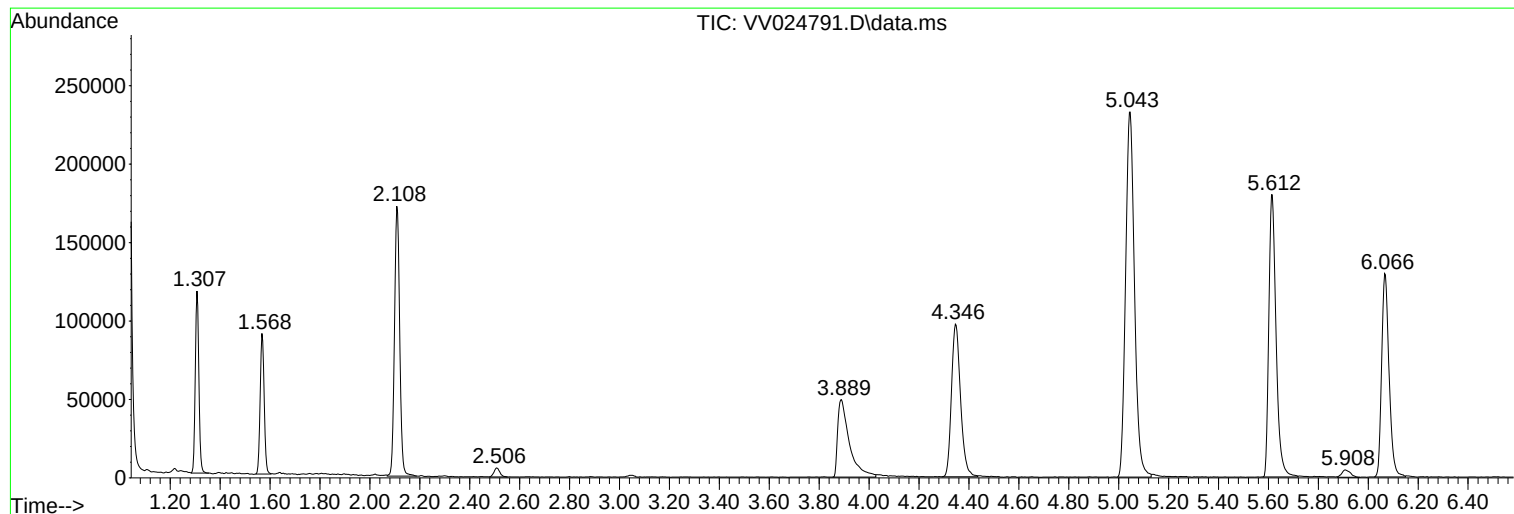

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022222\
Data File : VV024791.D
Acq On : 22 Feb 2022 12:35
Operator : SY/MD
Sample : VV0222WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK310

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022222\
Data File : VV024791.D
Acq On : 22 Feb 2022 12:35
Operator : SY/MD
Sample : VV0222WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK310

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
