

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022222\
 Data File : VV024795.D
 Acq On : 22 Feb 2022 14:22
 Operator : SY/MD
 Sample : N1623-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBD24

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV024795.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	97	rVB	120065	116971	20.00%	2.431%
2	1.568	156	164	179	rBV	89576	100808	17.24%	2.095%
3	2.111	322	333	354	rVB	170873	251078	42.93%	5.217%
4	3.902	876	890	918	rBV2	69925	254053	43.44%	5.279%
5	4.349	1013	1029	1057	rBV	99254	245685	42.01%	5.105%
6	5.050	1229	1247	1278	rBV2	235117	584819	100.00%	12.152%
7	5.619	1411	1424	1450	rBV	182033	369200	63.13%	7.672%
8	5.915	1501	1516	1547	rBV	105327	214633	36.70%	4.460%
9	6.069	1552	1564	1593	rBV	130902	269326	46.05%	5.596%
10	6.989	1840	1850	1874	rBV	59915	111151	19.01%	2.310%
11	7.317	1939	1952	1986	rBV	288154	505462	86.43%	10.503%
12	7.625	2037	2048	2072	rBV	32241	58465	10.00%	1.215%
13	7.982	2151	2159	2169	rVB5	4492	7852	1.34%	0.163%
14	8.088	2182	2192	2233	rBV	203687	397362	67.95%	8.257%
15	8.850	2418	2429	2448	rBV	266491	435585	74.48%	9.051%
16	10.214	2840	2853	2869	rBV	74532	117108	20.02%	2.433%
17	10.384	2898	2906	2916	rVB3	4294	6533	1.12%	0.136%
18	11.246	3163	3174	3196	rBV	254979	397143	67.91%	8.252%
19	11.622	3280	3291	3310	rBV	230956	363186	62.10%	7.547%
20	13.519	3872	3881	3890	rBV4	4561	6196	1.06%	0.129%




Sum of corrected areas: 4812616

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022222\
Data File : VV024795.D
Acq On : 22 Feb 2022 14:22
Operator : SY/MD
Sample : N1623-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBD24

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

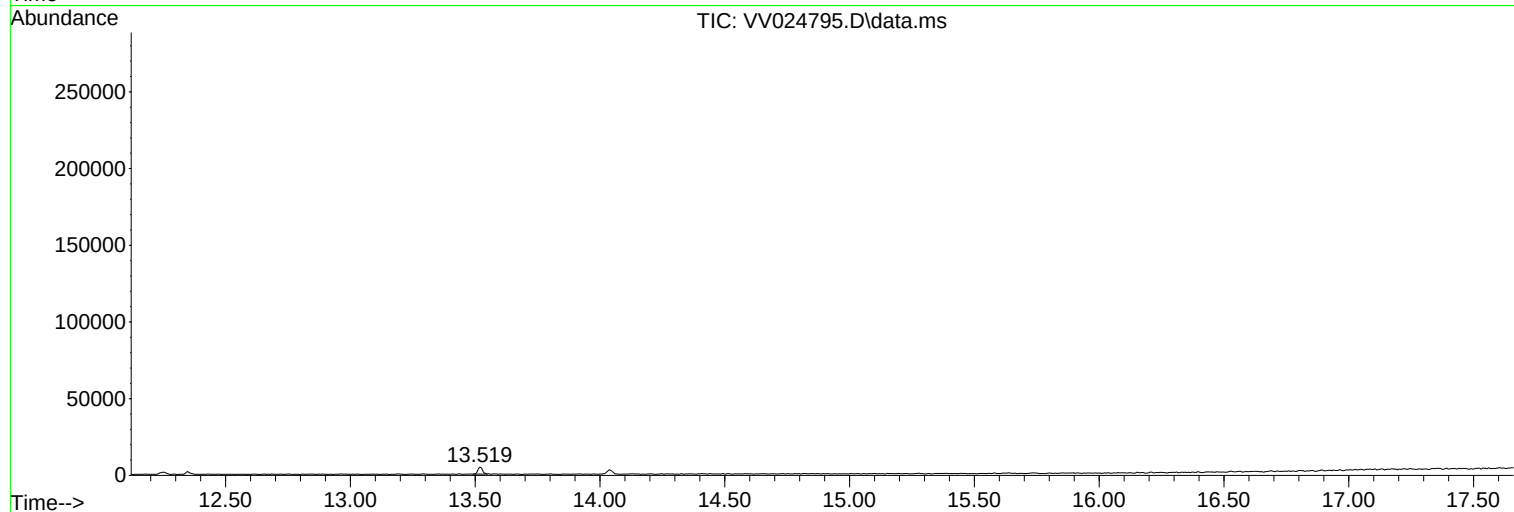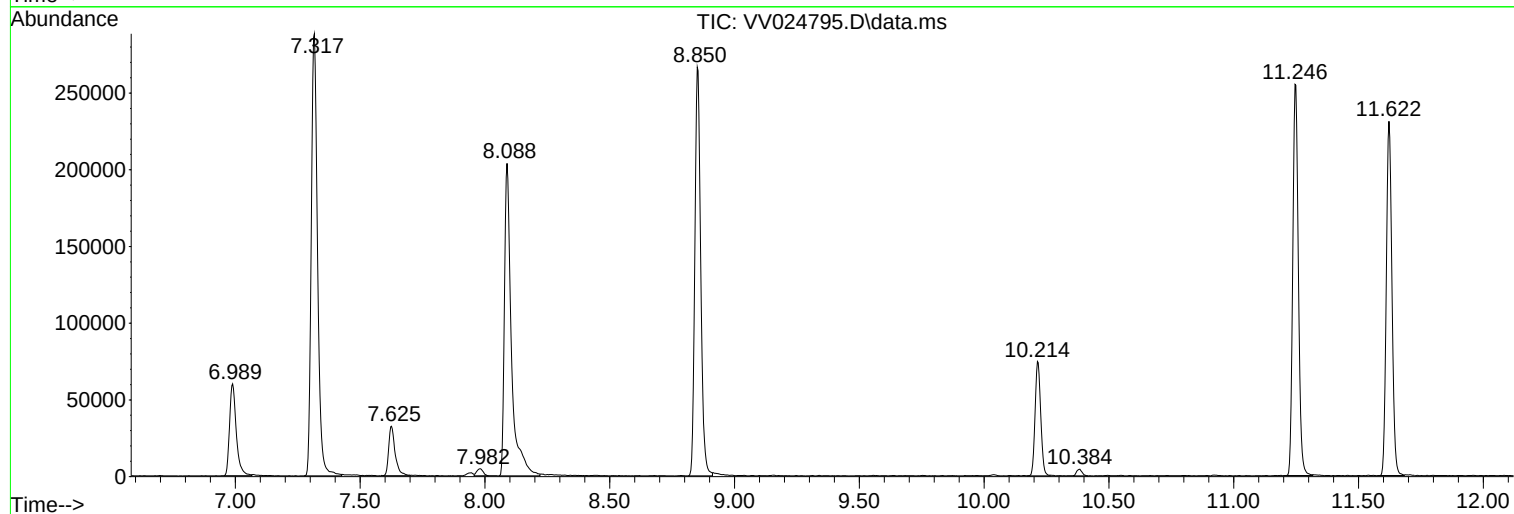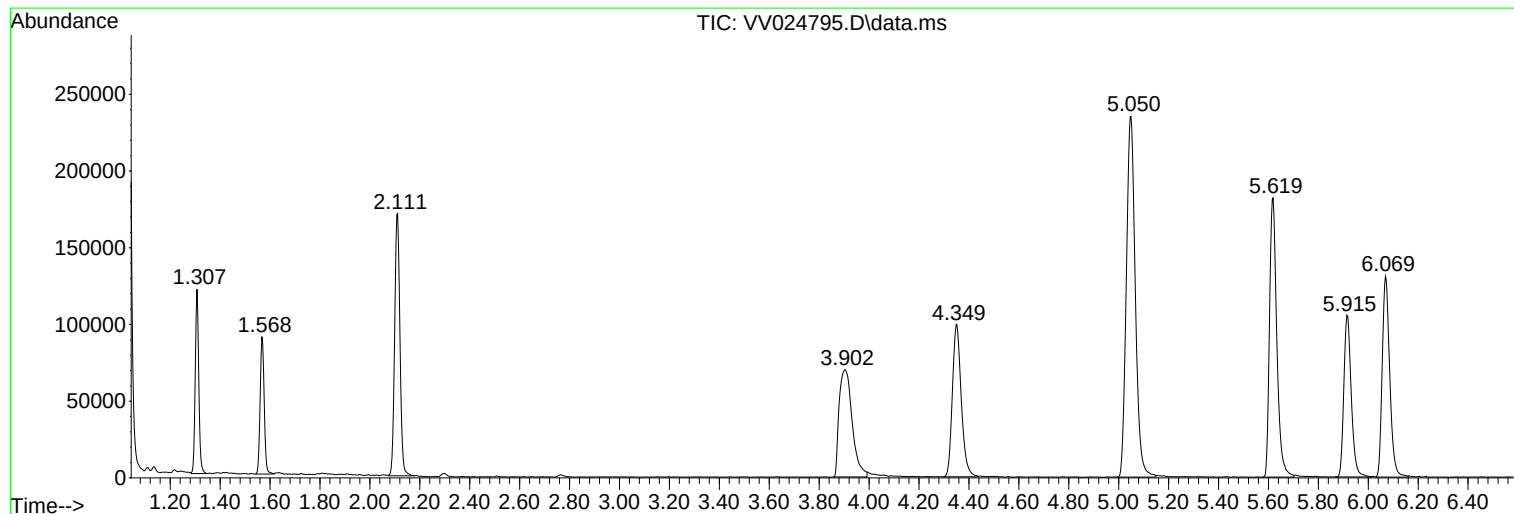

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022222\
Data File : VV024795.D
Acq On : 22 Feb 2022 14:22
Operator : SY/MD
Sample : N1623-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBD24










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.989	1.51 ug/L	111151	1,4-Difluorobenzene	5.619

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	3-Thiatricyclo[3.1.1.0(2,4)]heptane	112	C6H8S	1000221-37-0	47		
2	Thiophosgene	114	CCl2S	000463-71-8	42		
3	Methane, oxybis[chloro-	114	C2H4Cl2O	000542-88-1	33		
4	Methane, oxybis[chloro-	114	C2H4Cl2O	000542-88-1	33		
5	2-Propanol, 1,3-dichloro-	128	C3H6Cl2O	000096-23-1	28		

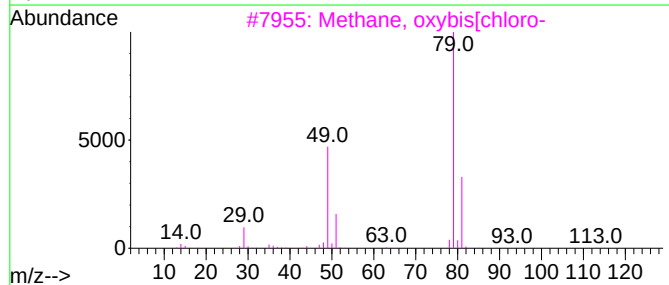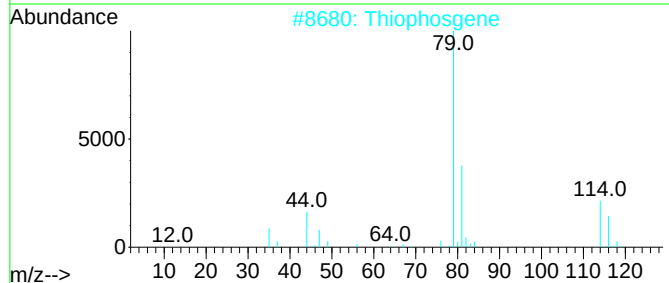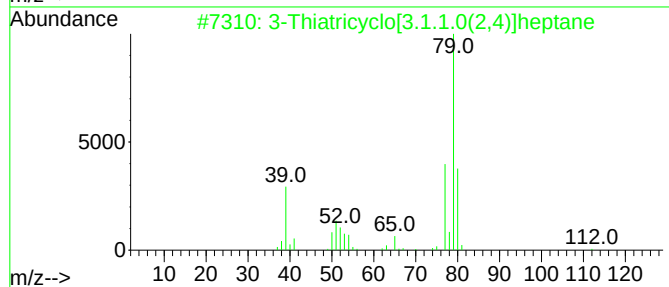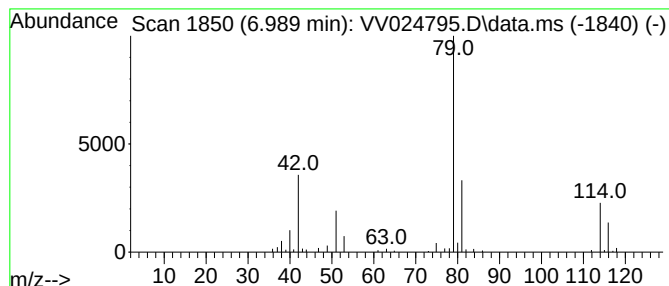

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022222\
Data File : VV024795.D
Acq On : 22 Feb 2022 14:22
Operator : SY/MD
Sample : N1623-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBD24

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	6.989	1.5	ug/L	111151	1	5.619	369200	5.0