
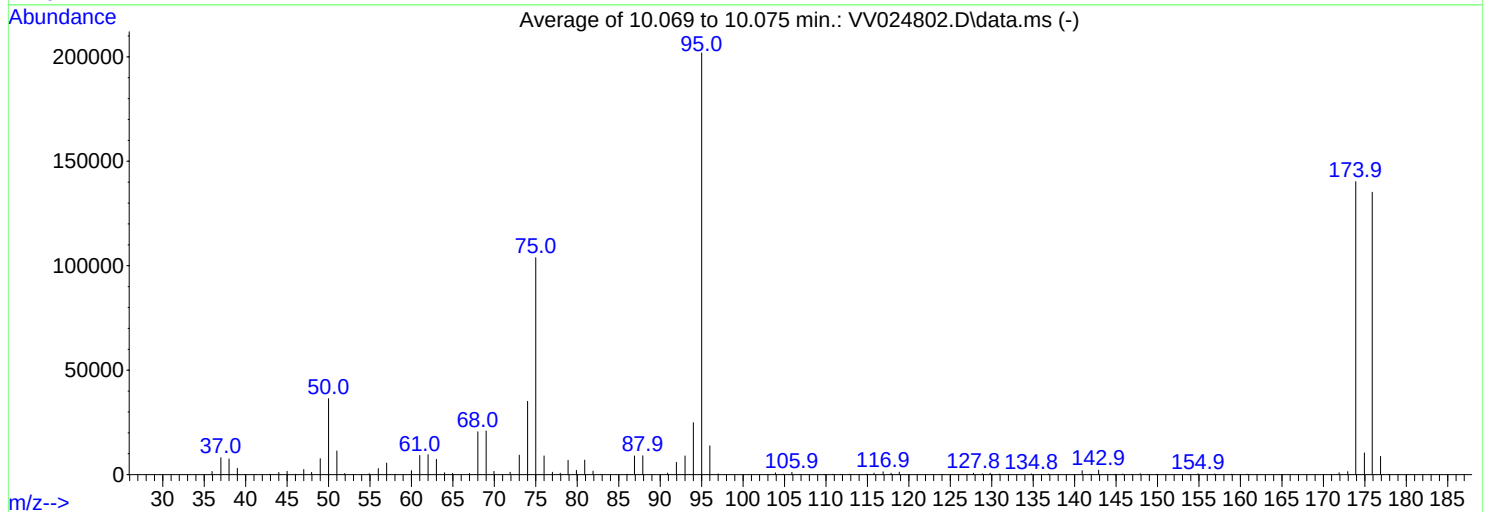


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022322\
 Data File : VV024802.D
 Acq On : 23 Feb 2022 09:30
 Operator : SY/MD
 Sample : BFB211
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB211

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM022322.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu Feb 24 00:58:52 2022

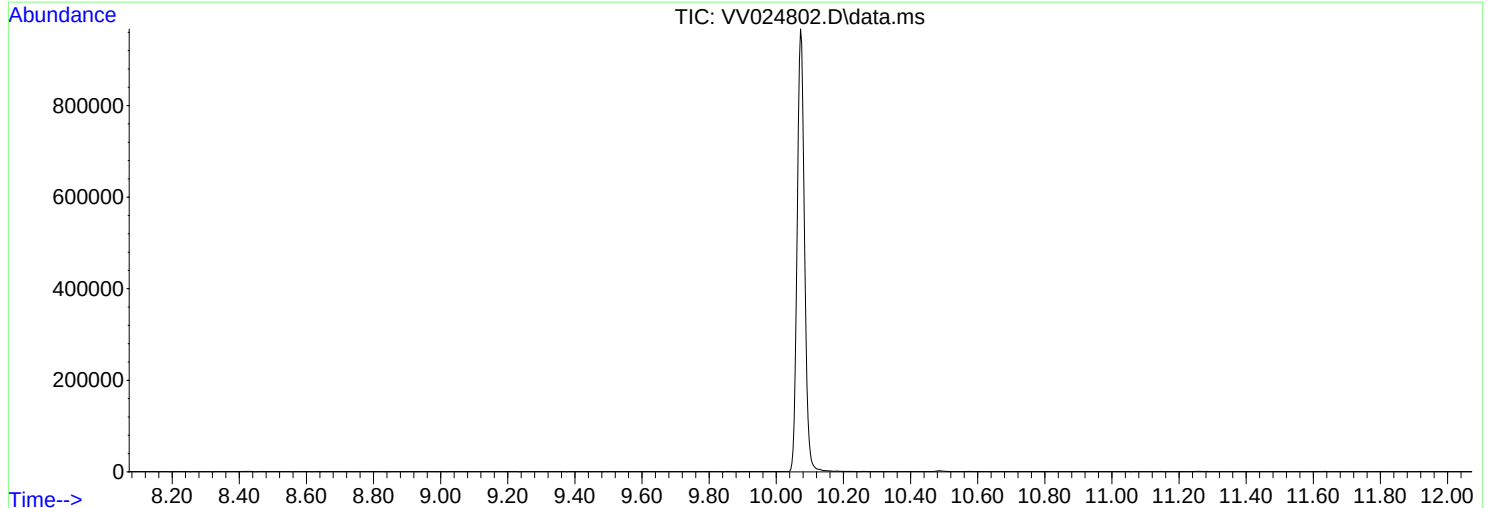

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	36411	PASS
75	95	30	80	51.5	103885	PASS
95	95	100	100	100.0	201899	PASS
96	95	5	9	6.8	13828	PASS
173	174	0.00	2	1.0	1452	PASS
174	95	50	120	69.5	140224	PASS
175	174	5	9	7.4	10431	PASS
176	174	95	101	96.4	135197	PASS
177	176	5	9	6.4	8700	PASS

m/z	Abundance
40.00	327.0
44.00	310.0

Instrument :
MSVOA_V
ClientSampleId :
BFB211

m/z	Abundance
35.90	1543.0
37.00	7978.0
38.00	7351.0
39.00	3069.0
39.90	339.0
42.90	107.0
44.00	1405.0
45.00	1454.0
46.00	184.0
47.00	2459.0
47.90	1023.0
49.00	7570.0
50.00	35768.0
51.00	11118.0
51.90	547.0
52.90	128.0
54.90	476.0
56.00	2849.0
57.00	5349.0
58.00	249.0
60.00	1902.0
61.00	9102.0
62.00	9328.0
63.00	7301.0
64.00	884.0
65.00	673.0
67.00	477.0
68.00	19896.0
69.00	20448.0
70.00	1655.0
71.90	960.0
73.00	9016.0
74.00	34448.0
75.00	101080.0
76.00	8750.0
77.00	1157.0
78.00	664.0
78.90	6762.0
79.90	2026.0
80.90	6628.0
81.90	1643.0
82.90	135.0
86.00	231.0
86.90	8955.0
87.90	8717.0
90.90	701.0
92.00	5590.0
93.00	8497.0
94.00	23984.0
95.00	194560.0
96.00	13278.0
97.00	408.0
103.90	796.0
104.90	266.0
105.90	990.0
106.80	135.0
109.80	128.0
110.90	173.0
111.70	214.0
112.80	235.0
114.80	264.0
115.80	763.0
116.90	1319.0
117.80	687.0
118.80	1118.0
127.80	752.0
128.90	359.0
129.80	685.0
130.90	281.0
134.80	385.0
136.80	286.0
140.90	1821.0
141.90	250.0
142.90	2076.0
143.80	147.0
144.80	288.0
145.80	273.0
146.90	156.0
147.90	419.0
148.80	122.0
149.90	171.0
153.00	138.0
153.80	131.0
154.90	530.0
156.90	379.0
158.90	199.0
160.90	200.0
171.00	134.0
171.90	935.0
173.00	1392.0
173.90	131968.0
174.90	9913.0

Instrument :
MSVOA_V
ClientSampleId :
BFB211

175.90127000.0

176.908227.0

177.90243.0

Instrument :
MSVOA_V

ClientSampleId :
BFB211

m/z	Abundance
35.90	1590.0
37.00	8389.0
38.00	7687.0
39.00	3174.0
39.90	382.0
42.90	100.0
44.00	1490.0
45.00	1660.0
46.00	218.0
47.00	2491.0
47.90	1085.0
49.00	7855.0
50.00	37696.0
51.00	11751.0
52.00	567.0
52.90	152.0
54.90	476.0
56.00	3043.0
57.00	5708.0
58.00	275.0
60.00	1963.0
61.00	9500.0
62.00	9810.0
63.00	7549.0
64.00	965.0
64.90	640.0
67.00	532.0
68.00	21288.0
69.00	21672.0
69.90	1668.0
71.90	1170.0
73.00	9647.0
74.00	36280.0
75.00	107448.0
76.00	9264.0
77.00	1224.0
77.90	743.0
78.90	7210.0
79.90	2139.0
80.90	7314.0
81.90	1714.0
82.90	162.0
86.00	192.0
86.90	9282.0
87.90	9377.0
90.90	782.0
92.00	6095.0
93.00	9268.0
94.00	25848.0
95.00	209408.0
96.00	14433.0
97.00	450.0
103.90	885.0
104.90	262.0
105.90	1088.0
106.90	163.0
109.90	153.0
110.90	228.0
111.70	213.0
112.80	214.0
114.80	285.0
115.80	820.0
116.90	1485.0
117.90	722.0
118.80	1272.0
123.90	103.0
127.80	762.0
128.90	404.0
129.80	739.0
130.90	307.0
134.80	429.0
136.90	322.0
139.90	101.0
140.90	1940.0
141.90	269.0
142.90	2221.0
143.80	162.0
144.80	273.0
145.80	301.0
146.90	171.0
147.90	505.0
148.80	131.0
149.90	187.0
153.00	146.0
153.80	165.0
154.90	514.0
156.90	409.0
158.90	233.0
160.80	232.0
171.00	168.0
171.90	958.0
172.90	1503.0

Instrument :
MSVOA_V
ClientSampleId :
BFB211

173.90	144896.0
174.90	10776.0
175.90	140096.0
176.90	8932.0
177.90	240.0

Instrument :
MSVOA_V
ClientSampleId :
BFB211

m/z	Abundance
36.00	1441.0
37.00	8054.0
38.00	7391.0
39.00	2887.0
39.90	417.0
44.00	1393.0
45.00	1660.0
46.10	216.0
47.00	2342.0
48.00	1054.0
49.00	7510.0
50.00	35768.0
51.00	11186.0
52.00	502.0
53.00	137.0
54.90	433.0
56.00	2812.0
57.00	5436.0
58.10	261.0
60.00	1859.0
61.00	8919.0
62.00	9540.0
63.00	7111.0
64.00	889.0
64.90	542.0
67.00	546.0
68.00	20328.0
69.00	20536.0
69.90	1501.0
71.90	1246.0
73.00	9312.0
74.00	34600.0
75.00	103128.0
76.00	8803.0
77.00	1145.0
77.90	798.0
78.90	6768.0
79.90	1945.0
80.90	7099.0
81.90	1658.0
82.80	196.0
86.00	184.0
86.90	8651.0
87.90	9104.0
90.90	803.0
91.90	6073.0
93.00	9047.0
94.00	24840.0
95.00	201728.0
96.00	13774.0
97.00	407.0
103.90	920.0
104.90	258.0
105.90	1078.0
106.90	195.0
109.90	166.0
110.80	249.0
111.80	166.0
112.90	179.0
114.90	251.0
115.80	769.0
116.90	1460.0
117.90	686.0
118.90	1213.0
123.90	138.0
127.80	679.0
128.90	406.0
129.80	700.0
130.90	280.0
134.80	388.0
136.80	325.0
140.90	1917.0
141.80	244.0
142.90	2141.0
143.80	138.0
144.90	250.0
145.80	281.0
146.90	145.0
147.90	524.0
148.80	123.0
149.90	180.0
153.00	140.0
153.80	165.0
154.90	459.0
156.90	377.0
158.90	218.0
160.70	247.0
170.80	164.0
171.90	899.0
172.90	1461.0
173.90	143808.0
175.00	10604.0

Instrument :
MSVOA_V
ClientSampleId :
BFB211

175.90	138496.0
176.90	8942.0
177.90	228.0

Instrument :
MSVOA_V
ClientSampleId :
BFB211