

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW022422\
 Data File : VW024815.D
 Acq On : 24 Feb 2022 11:56
 Operator : SY/MD
 Sample : N1623-20
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBD54

Quant Time: Feb 25 03:28:48 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Feb 25 03:28:05 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	162698	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	150404	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	64950	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	77039	5.583	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	111.600%
7) Chloroethane-d5	1.568	69	62835	5.550	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	111.000%
11) 1,1-Dichloroethene-d2	2.108	63	98297	3.887	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	77.800%
20) 2-Butanone-d5	3.889	46	114306	57.990	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	115.980%
24) Chloroform-d	4.346	84	120125	5.579	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	111.600%
26) 1,2-Dichloroethane-d4	5.027	65	54190	5.646	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	113.000%
32) Benzene-d6	5.047	84	252716	5.824	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	116.400%
36) 1,2-Dichloropropane-d6	6.066	67	75666	5.926	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	118.600%
41) Toluene-d8	7.313	98	215331	5.462	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	109.200%
43) trans-1,3-Dichloroprop...	7.619	79	22387	5.263	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	105.200%
46) 2-Hexanone-d5	8.085	63	79187	47.310	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	94.620%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	40726	5.292	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	105.800%
66) 1,2-Dichlorobenzene-d4	11.622	152	62525	5.564	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	111.200%
Target Compounds					Qvalue	
25) Chloroform	4.378	83	2317	0.098	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022422\
Data File : VV024815.D
Acq On : 24 Feb 2022 11:56
Operator : SY/MD
Sample : N1623-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBD54

Quant Time: Feb 25 03:28:48 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Feb 25 03:28:05 2022
Response via : Initial Calibration

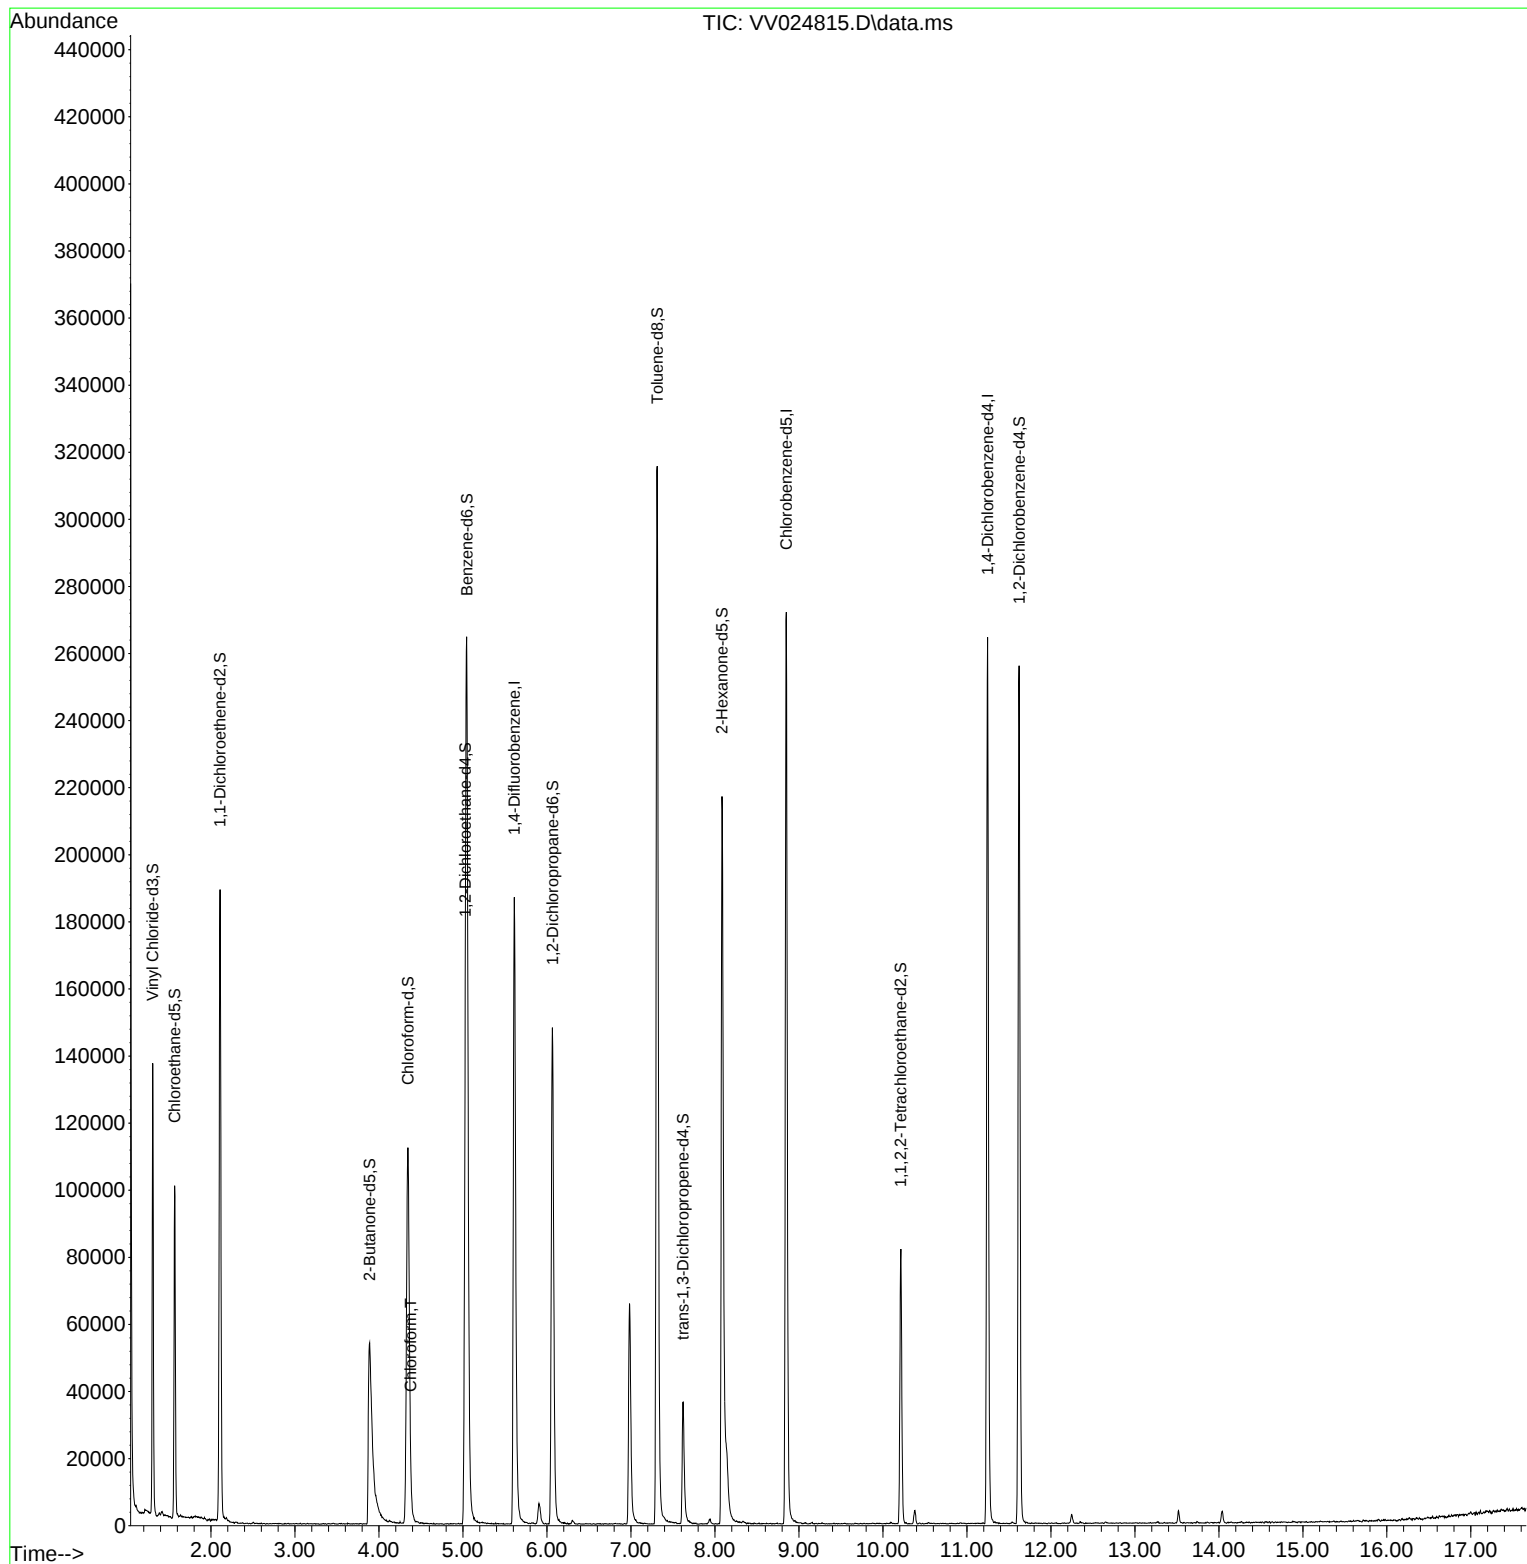

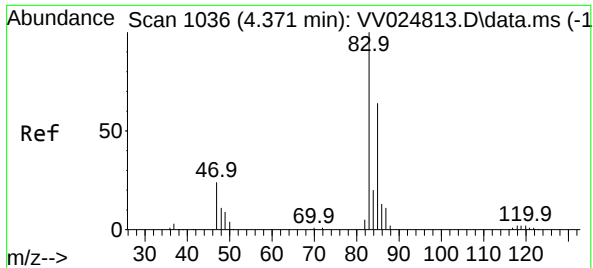

#25
 Chloroform
 Concen: 0.098 ug/L
 RT: 4.378 min Scan# 10
 Delta R.T. 0.006 min
 Lab File: VV024815.D
 Acq: 24 Feb 2022 11:56

Instrument :
 MSVOA_V
 ClientSampleId :
 GBD54

Tgt Ion: 83 Resp: 2317
 Ion Ratio Lower Upper
 83 100
 85 63.2 45.5 84.5

