

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW022422\
 Data File : VW024818.D
 Acq On : 24 Feb 2022 13:11
 Operator : SY/MD
 Sample : VIBLK260
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK260

Quant Time: Feb 25 03:29:27 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Feb 25 03:28:05 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	195143	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	174611	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	79477	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	80345	4.854	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	97.000%
7) Chloroethane-d5	1.568	69	65472	4.822	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	96.400%
11) 1,1-Dichloroethene-d2	2.108	63	103526	3.413	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	68.200%
20) 2-Butanone-d5	3.889	46	129641	54.834	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	109.660%
24) Chloroform-d	4.346	84	129576	5.017	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.400%
26) 1,2-Dichloroethane-d4	5.031	65	58862	5.113	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.200%
32) Benzene-d6	5.047	84	280418	5.567	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	111.400%
36) 1,2-Dichloropropane-d6	6.066	67	83055	5.603	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	112.000%
41) Toluene-d8	7.313	98	242316	5.294	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	105.800%
43) trans-1,3-Dichloroprop...	7.622	79	24761	5.014	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	100.200%
46) 2-Hexanone-d5	8.085	63	96596	49.710	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	99.420%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	47503	5.317	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	106.400%
66) 1,2-Dichlorobenzene-d4	11.622	152	73228	5.325	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	106.400%
Target Compounds					Qvalue	
25) Chloroform	4.365	83	2593	0.091	ug/L	80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022422\
Data File : VV024818.D
Acq On : 24 Feb 2022 13:11
Operator : SY/MD
Sample : VIBLK260
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK260

Quant Time: Feb 25 03:29:27 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Feb 25 03:28:05 2022
Response via : Initial Calibration

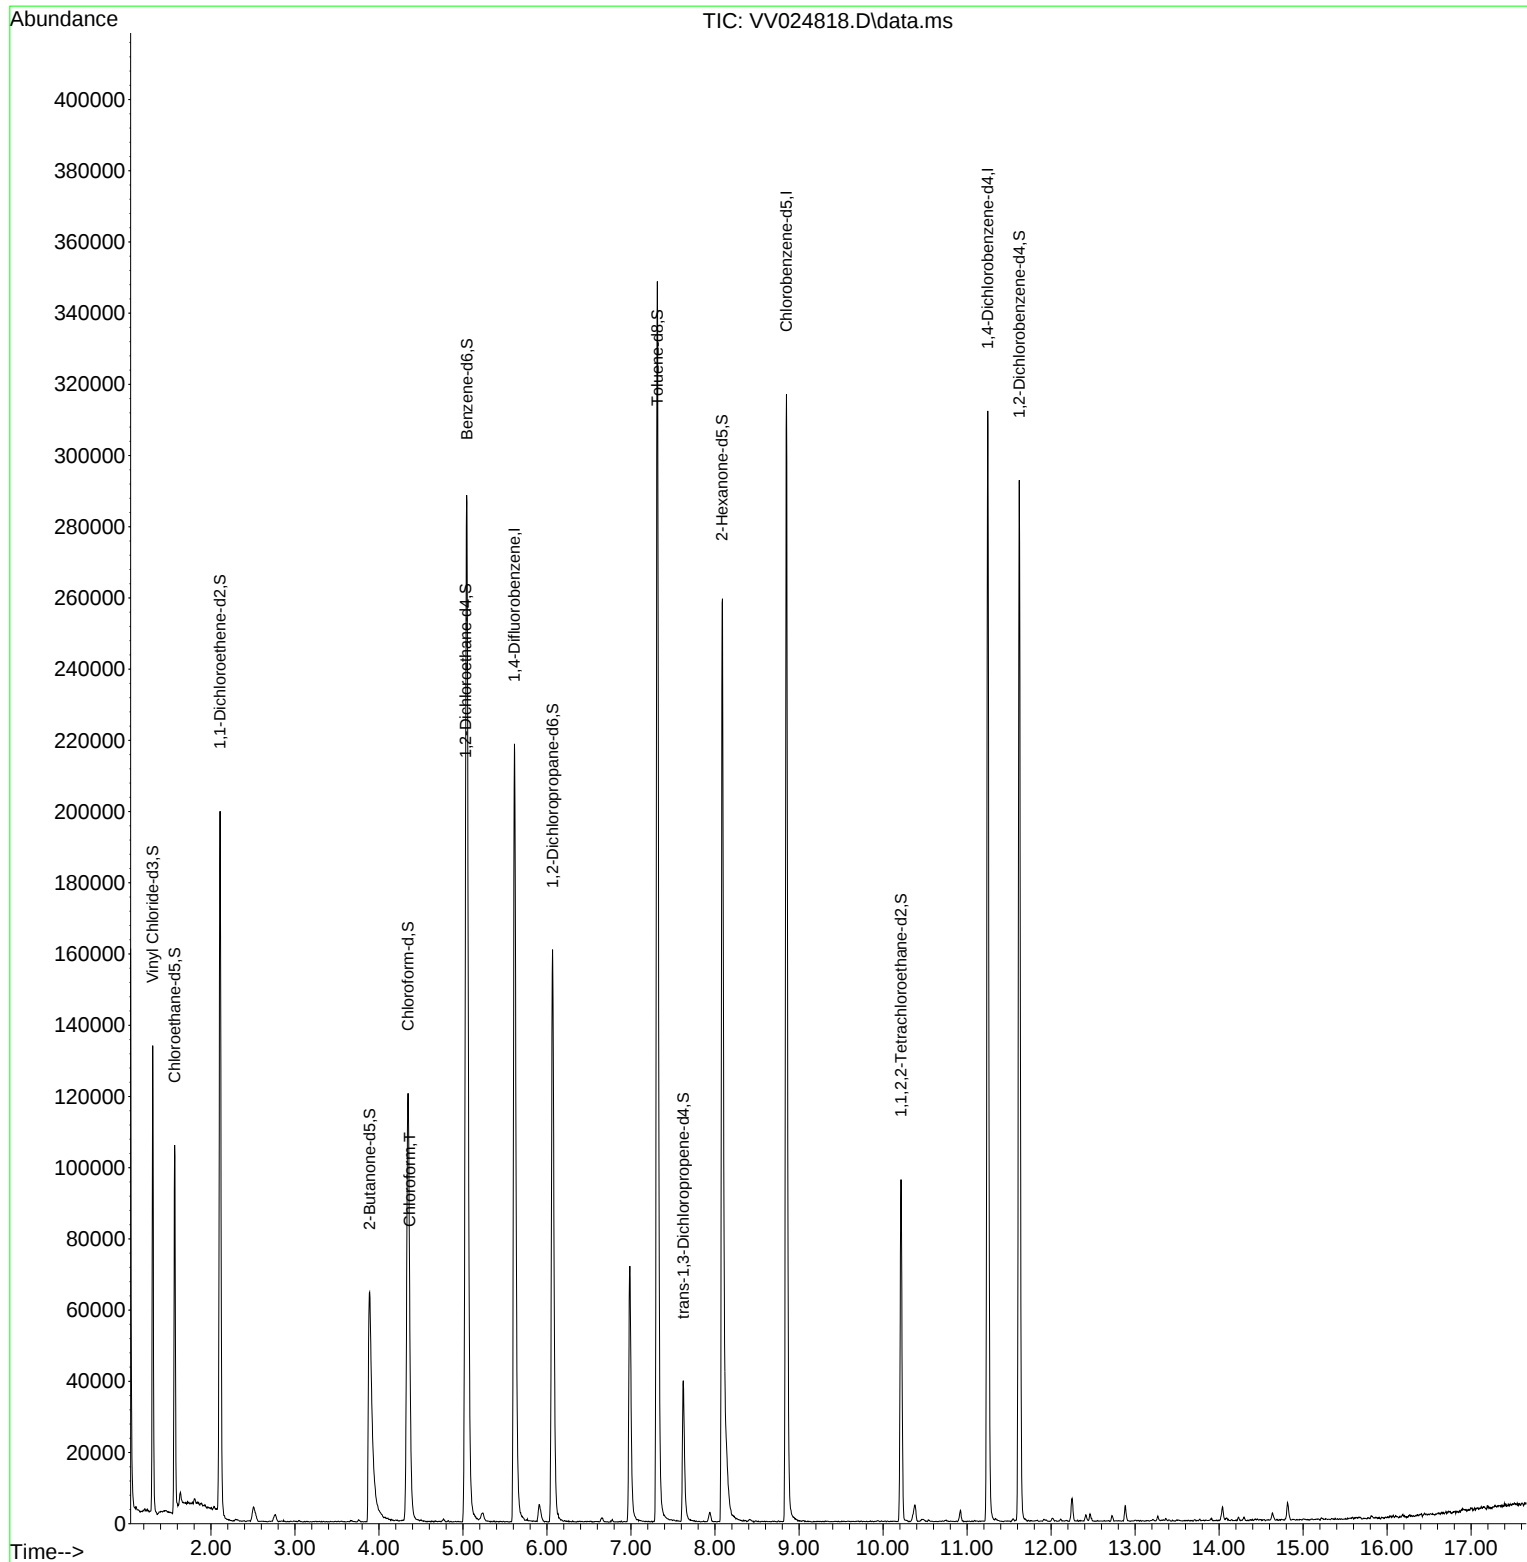

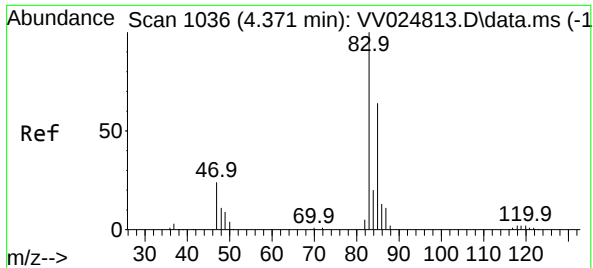

#25
 Chloroform
 Concen: 0.091 ug/L
 RT: 4.365 min Scan# 10
 Delta R.T. -0.006 min
 Lab File: VV024818.D
 Acq: 24 Feb 2022 13:11

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK260

Tgt Ion: 83 Resp: 2593
 Ion Ratio Lower Upper
 83 100
 85 80.9 45.5 84.5

