

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022422\
 Data File : VV024820.D
 Acq On : 24 Feb 2022 15:36
 Operator : SY/MD
 Sample : N1623-19
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Feb 25 03:29:51 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Feb 25 03:28:05 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	187069	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	170137	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	72838	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	67692	4.266	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	85.400%	
7) Chloroethane-d5	1.568	69	57798	4.440	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	88.800%	
11) 1,1-Dichloroethene-d2	2.108	63	89987	3.095	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	61.800%	
20) 2-Butanone-d5	3.886	46	110218	48.631	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	97.260%	
24) Chloroform-d	4.346	84	112177	4.531	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	90.600%	
26) 1,2-Dichloroethane-d4	5.027	65	49647	4.499	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	90.000%	
32) Benzene-d6	5.047	84	237939	4.848	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	97.000%	
36) 1,2-Dichloropropane-d6	6.066	67	70950	4.912	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	98.200%	
41) Toluene-d8	7.313	98	203980	4.574	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	91.400%	
43) trans-1,3-Dichloroprop...	7.622	79	21047	4.374	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	87.400%	
46) 2-Hexanone-d5	8.085	63	78590	41.507	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	83.020%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	39917	4.585	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	91.800%	
66) 1,2-Dichlorobenzene-d4	11.622	152	60515	4.802	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	96.000%	
Target Compounds					Qvalue	
25) Chloroform	4.371	83	2791	0.103	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022422\
Data File : VV024820.D
Acq On : 24 Feb 2022 15:36
Operator : SY/MD
Sample : N1623-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Time: Feb 25 03:29:51 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Feb 25 03:28:05 2022
Response via : Initial Calibration

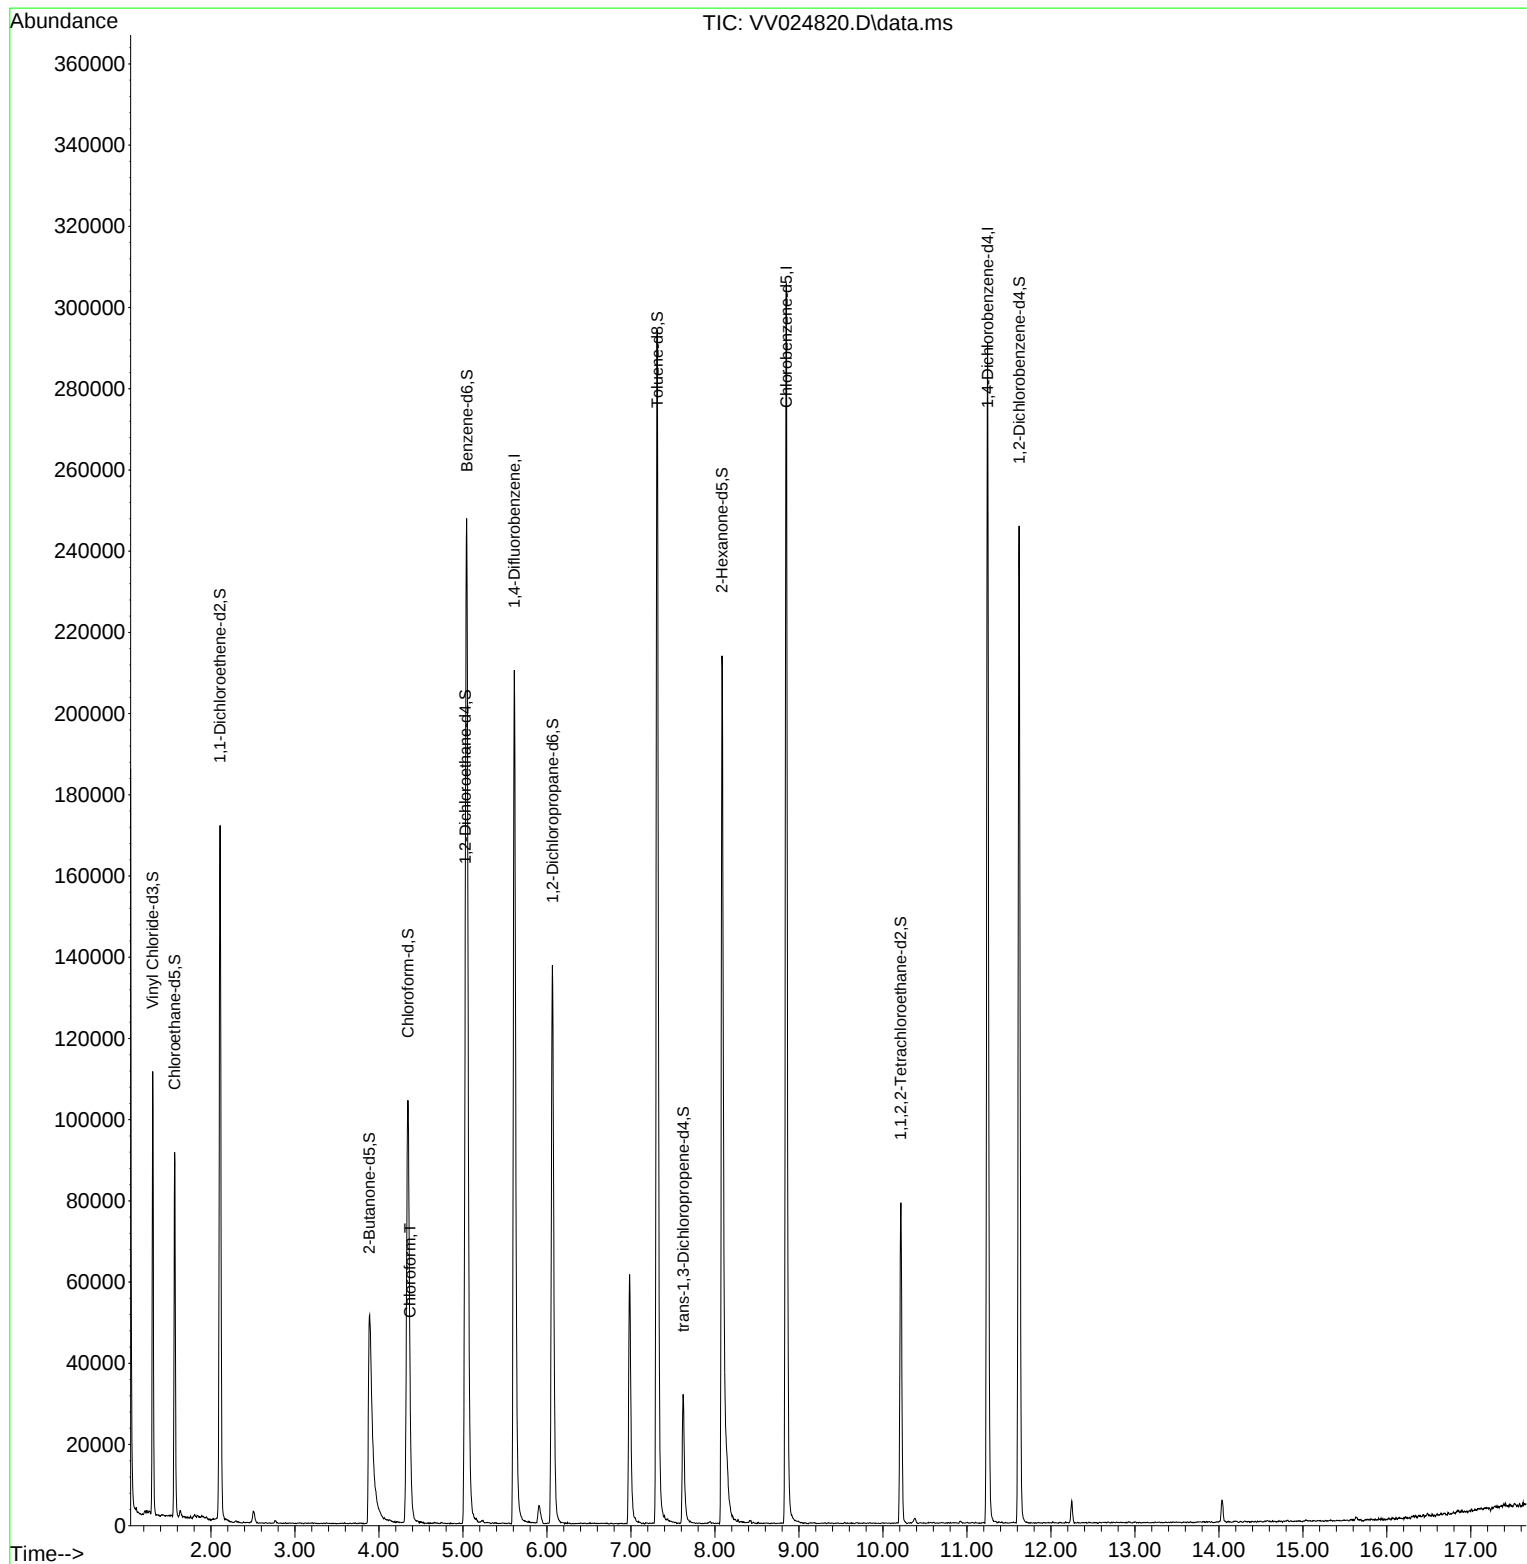

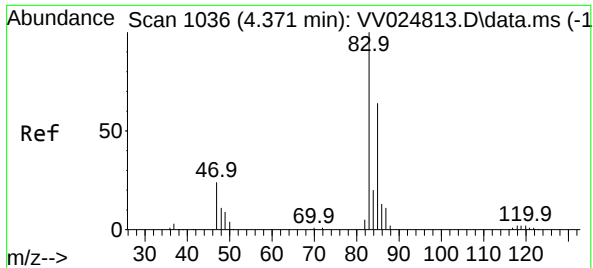

#25

Chloroform

Concen: 0.103 ug/L

RT: 4.371 min Scan# 10

Delta R.T. 0.000 min

Lab File: VV024820.D


Acq: 24 Feb 2022 15:36

Instrument :

MSVOA_V

ClientSampleId :

VHBLK001

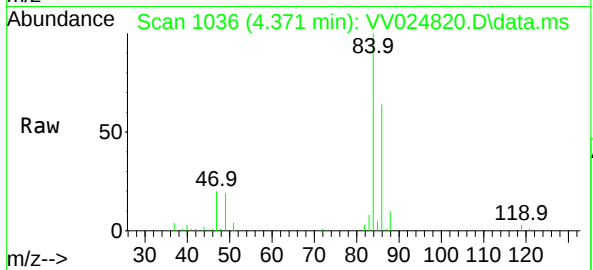

Tgt Ion: 83 Resp: 2791

Ion Ratio Lower Upper

83 100

85 69.5 45.5 84.5

