

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022422\
 Data File : VV024820.D
 Acq On : 24 Feb 2022 15:36
 Operator : SY/MD
 Sample : N1623-19
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV024820.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	95	rVB	109291	109295	17.90%	2.266%
2	1.568	156	164	178	rVB	89799	101777	16.66%	2.111%
3	2.108	321	332	350	rVB	170983	244875	40.10%	5.078%
4	3.889	874	886	938	rBV	51331	178894	29.29%	3.710%
5	4.346	1012	1028	1059	rBV2	103972	263002	43.06%	5.454%
6	5.043	1226	1245	1278	rBV2	247548	610734	100.00%	12.665%
7	5.612	1411	1422	1456	rBV	210225	427098	69.93%	8.857%
8	5.905	1505	1513	1531	rVB5	4447	10272	1.68%	0.213%
9	6.066	1550	1563	1588	rBV	137395	281112	46.03%	5.830%
10	6.985	1839	1849	1875	rBV	61353	112699	18.45%	2.337%
11	7.313	1939	1951	1976	rBV	293950	519059	84.99%	10.764%
12	7.622	2035	2047	2070	rBV2	31844	58890	9.64%	1.221%
13	8.085	2182	2191	2228	rBV	213722	428955	70.24%	8.895%
14	8.850	2417	2429	2460	rBV	305383	500462	81.94%	10.378%
15	10.214	2843	2853	2868	rBV	78880	124703	20.42%	2.586%
16	11.246	3164	3174	3195	rBV	290848	451117	73.86%	9.355%
17	11.622	3280	3291	3316	rBV	245549	383581	62.81%	7.954%
18	12.249	3475	3486	3495	rVB	5487	7811	1.28%	0.162%
19	14.037	4035	4042	4054	rVB2	5164	7862	1.29%	0.163%




Sum of corrected areas: 4822198

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022422\
Data File : VV024820.D
Acq On : 24 Feb 2022 15:36
Operator : SY/MD
Sample : N1623-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

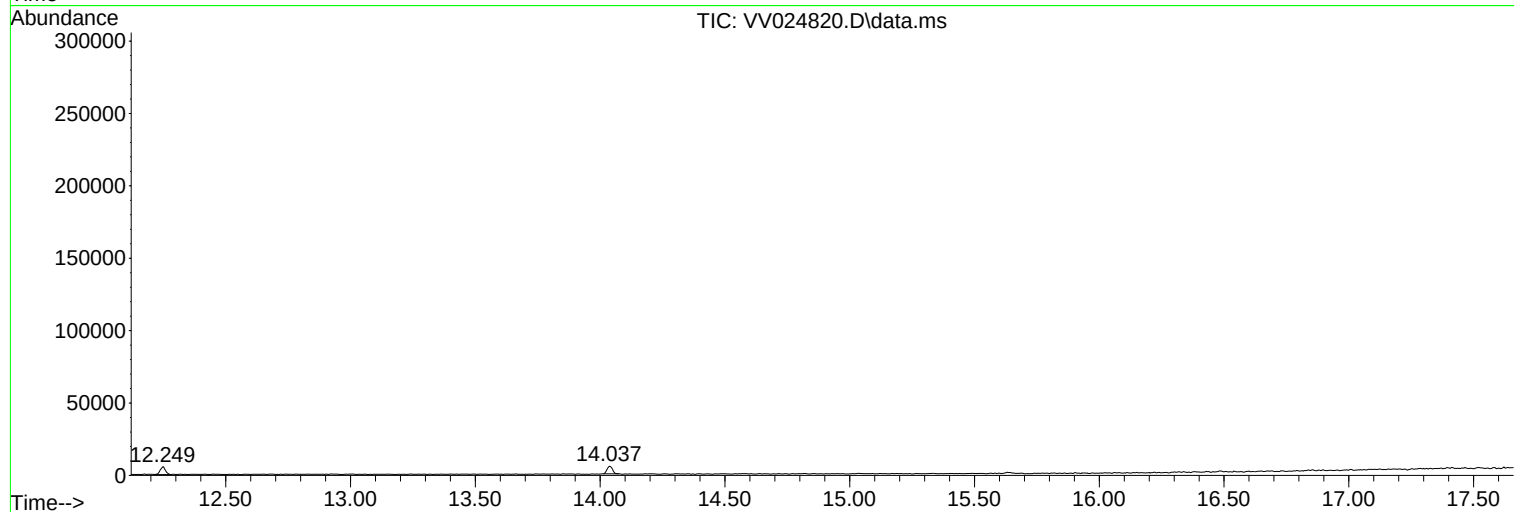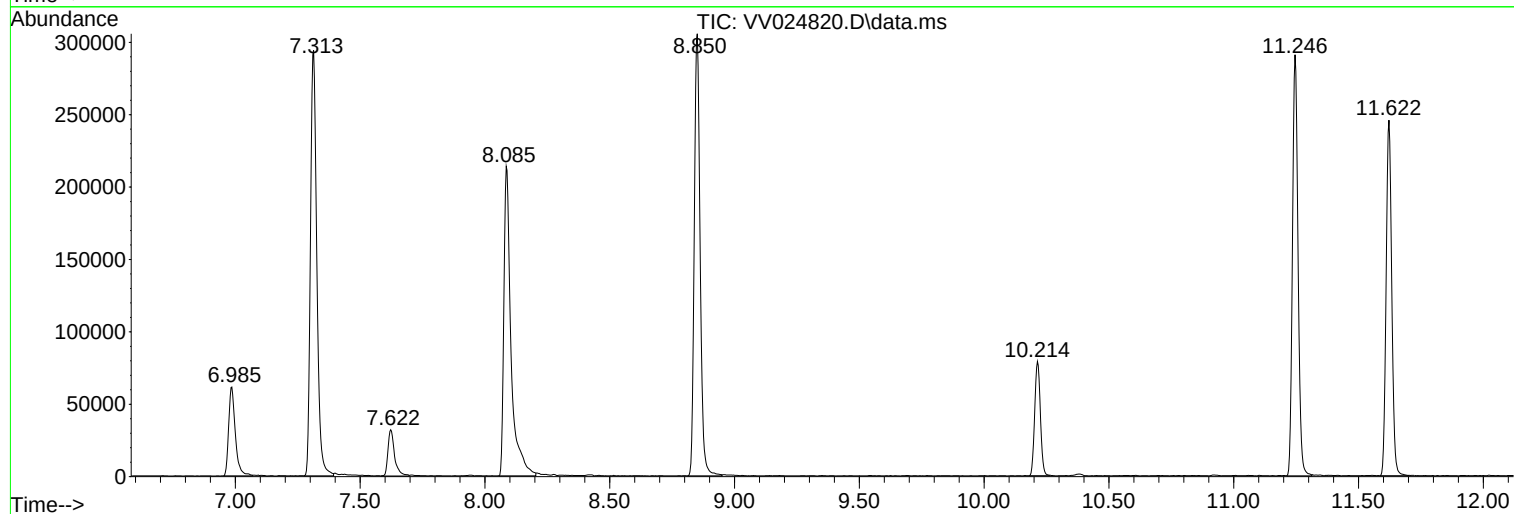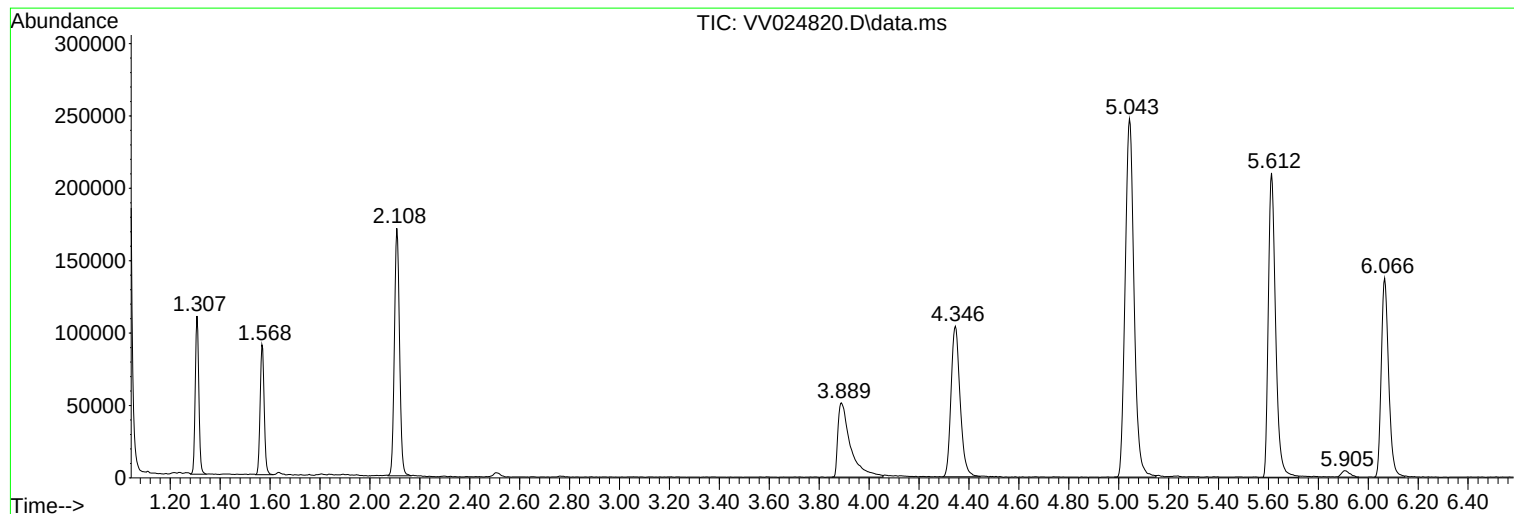

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022422\
Data File : VV024820.D
Acq On : 24 Feb 2022 15:36
Operator : SY/MD
Sample : N1623-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022422\
Data File : VV024820.D
Acq On : 24 Feb 2022 15:36
Operator : SY/MD
Sample : N1623-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------