

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW022724\
 Data File : VW034445.D
 Acq On : 27 Feb 2024 13:34
 Operator : SY/MD
 Sample : P1566-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 JWAC6

Quant Time: Feb 28 03:56:15 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022624WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Feb 28 03:52:36 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.538	114	137553	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	131474	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	65746	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	36239	4.538	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	90.800%
7) Chloroethane-d5	1.532	69	32751	4.644	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	92.800%
11) 1,1-Dichloroethene-d2	2.059	65	17249	4.641	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	92.800%
20) 2-Butanone-d5	3.802	46	103034	49.354	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	98.700%
24) Chloroform-d	4.252	84	78889	4.921	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.400%
26) 1,2-Dichloroethane-d4	4.947	65	42796	5.245	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	105.000%
32) Benzene-d6	4.963	84	137929	4.664	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.200%
36) 1,2-Dichloropropane-d6	5.992	67	44474	5.036	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.800%
41) Toluene-d8	7.246	98	120346	4.537	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.800%
43) trans-1,3-Dichloroprop...	7.561	79	15655	4.758	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	95.200%
46) 2-Hexanone-d5	8.024	63	98078	52.723	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	105.440%
56) 1,1,2,2-Tetrachloroeth...	10.156	84	35935	5.141	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	102.800%
66) 1,2-Dichlorobenzene-d4	11.561	152	51428	5.149	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.000%
Target Compounds						Qvalue
13) Acetone	2.130	43	20903	9.844	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022724\
Data File : VV034445.D
Acq On : 27 Feb 2024 13:34
Operator : SY/MD
Sample : P1566-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JWAC6

Quant Time: Feb 28 03:56:15 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022624WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Feb 28 03:52:36 2024
Response via : Initial Calibration

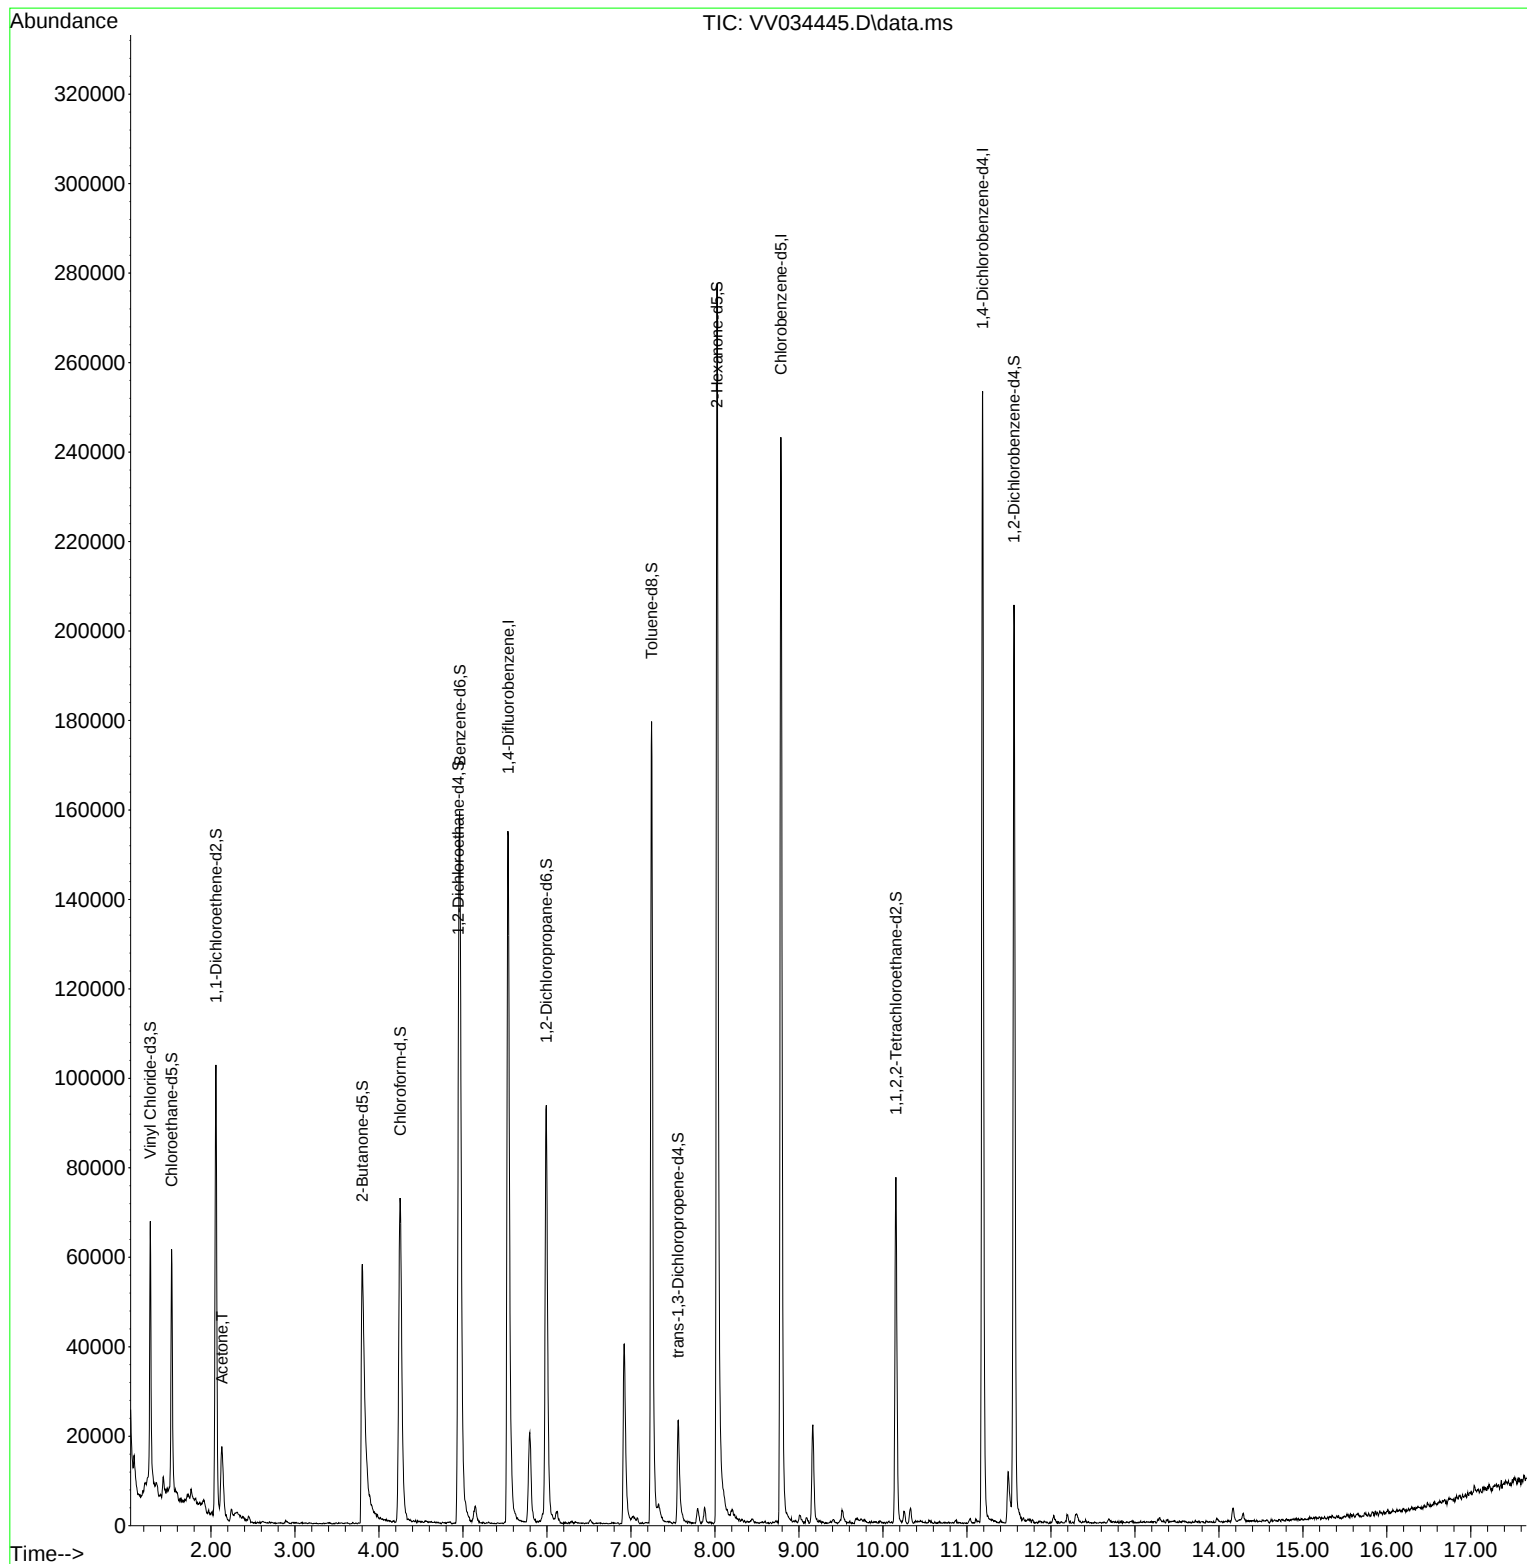

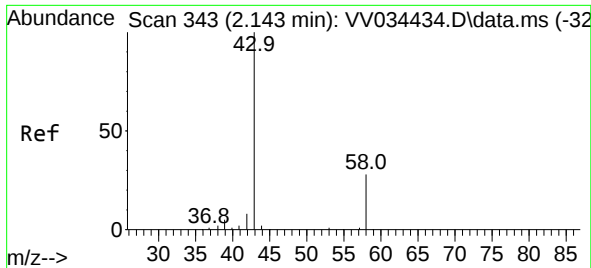

#13

Acetone

Concen: 9.844 ug/L

RT: 2.130 min Scan# 31

Delta R.T. -0.013 min

Lab File: VV034445.D


Acq: 27 Feb 2024 13:34

Instrument :

MSVOA_V

ClientSampleId :

JWAC6

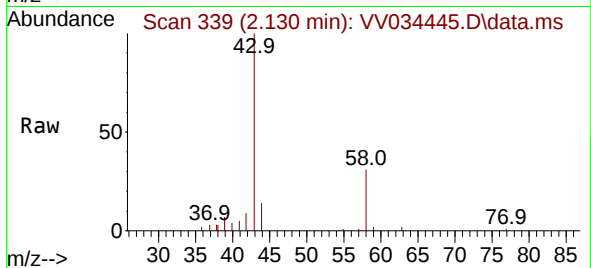

Tgt Ion: 43 Resp: 20903

Ion Ratio Lower Upper

43 100

58 31.9 0.0 56.2

